


DULCOMETER® D1Cb / D1Cc



**D1Cc**

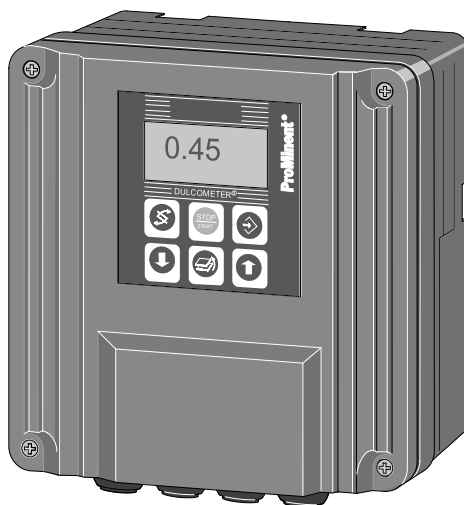

**D1Cb**

**Please carefully read these operating instructions before use! · Do not discard!  
The operator shall be liable for any damage caused by installation or operating errors!  
Technical changes reserved.**

ProMinent Dosiertechnik GmbH  
Im Schuhmachergewann 5 - 11  
69123 Heidelberg  
Telephone: +49 6221 842-0  
Fax: +49 6221 842-419  
email: [info@prominent.de](mailto:info@prominent.de)  
Internet: [www.prominent.com](http://www.prominent.com)

986362, 4, en\_GB

### General non-discriminatory approach

In order to make it easier to read, this document uses the male form in grammatical structures but with an implied neutral sense. It is aimed equally at both men and women. We kindly ask female readers for their understanding in this simplification of the text.

### Supplementary information

Read the following supplementary information in its entirety!

The following are highlighted separately in the document:

■ Enumerated lists

—▶ Instructions

⇒ Results of the instructions

### Information



*This provides important information relating to the correct operation of the system or is intended to make your work easier.*

### Safety information

Safety information are provided with detailed descriptions of the endangering situation, see ↪ *Chapter 1.1 'Explanation of the safety information' on page 8*

# Table of contents

<b>1</b>	<b>Introduction.....</b>	<b>8</b>
1.1	Explanation of the safety information.....	8
1.2	Users' qualifications.....	10
1.3	General Safety Information.....	11
1.4	Correct and proper use.....	13
1.5	ID Code.....	14
<b>2</b>	<b>Functional description.....</b>	<b>17</b>
2.1	Wall mounting/control panel installation.....	18
2.2	Electrical construction.....	19
2.2.1	Block circuit diagram.....	20
2.2.2	Galvanic Isolation .....	21
<b>3</b>	<b>D1Cb mounting.....</b>	<b>22</b>
3.1	Scope of supply.....	23
3.2	Installation (Wall Mounted) .....	24
3.3	Installation - Control Panel Mounted (Optional) .....	25
3.4	Wall Mounted Installation of D1Cb (Electrical) .....	27
3.4.1	Opening the device.....	28
3.4.2	Electrical Installation (Wall Mounted) .....	29
3.4.3	Electrical Installation (Control Panel Mounted) .....	30
3.4.4	Installation of Coaxial Cable to Guard Terminal XE1 .....	31
3.4.5	Cable Cross-Sections and Cable End Sleeves.....	32
3.4.6	Protective RC Circuit (Optional) .....	33
3.4.7	Terminal Wiring Diagram .....	34
3.5	Switching of inductive loads.....	38
<b>4</b>	<b>D1Cc mounting.....</b>	<b>40</b>
4.1	DULCOMETER® D1Cc scope of supply.....	41
4.2	Mounting - control panel installation DULCOMETER® D1Cc.....	41
4.3	Electrical Installation (Control Panel Mounted).....	44
4.3.1	Installation of Coaxial Cable to Guard Terminal XE1.....	45
4.3.2	Cable Cross-Sections and Cable End Sleeves.....	47
4.3.3	Terminal diagram .....	48
4.4	Switching of inductive loads.....	50

<b>5</b>	<b>Commissioning</b> .....	<b>52</b>
5.1	Initial commissioning .....	52
5.1.1	Selection of the Operating Language.....	52
5.1.2	Selection of the Measured Variable and Measuring Range.....	54
5.2	Activation Code for Extended Functions.....	55
5.2.1	Extended Functions Obtainable with the Activation Code.....	55
<b>6</b>	<b>Operating diagram/ Display Symbols</b> .....	<b>59</b>
6.1	Overview of equipment/Control elements.....	59
6.2	Display Symbols.....	60
6.3	Permanent Display 1 .....	61
6.4	Continuous display 2.....	62
6.5	Continuous display 3.....	62
6.6	Operating diagram.....	64
6.7	Reduced / Complete Operating Menu .....	67
6.8	Fault Messages.....	67
6.8.1	Fault display.....	67
6.9	General settings.....	68
6.9.1	Access code.....	68
<b>7</b>	<b>Measured Variables and Operating Menus for Amperometric Sensors</b> .....	<b>69</b>
7.1	Reduced / Complete Operating Menu .....	70
7.2	Description of All Amperometric Measured Variables .....	70
7.3	Reduced Operating Menu .....	71
7.4	Complete Operating Menu / Description of All Measured Variables.....	73
7.5	Calibration of All Amperometric Measured Variables .....	74
7.6	Calibration of the Sensor for Amperometric Measured Variables.....	75
7.6.1	Preparation for Calibration of the Sensors for Amperometric Measured Variables .....	75
7.6.2	Calibration of Zero Point and Slope.....	76
7.7	Setting the Measured value.....	79
7.8	Correcting value.....	79
<b>8</b>	<b>Measured Variables and Operating Menus for Potentiometric Sensors</b> .....	<b>81</b>
8.1	Reduced / Complete Operating Menu .....	82
8.2	Description of pH, Redox and Fluoride Measured Variables .....	82
8.3	Reduced pH / Redox / Fluoride Operating Menu .....	83
8.4	Complete Operating Menu/Description of pH / ORP / Fluoride.....	85
8.5	Calibration of pH, ORP and Fluoride Sensors.....	87

---

## Table of contents

---

8.5.1	Description of the Calibration of pH Sensors .....	88
8.5.2	Calibration of pH Sensors. Description of the Setting Ranges .....	91
8.5.3	Calibration of pH Sensors. Description of the Error Messages .....	91
8.5.4	Testing the Redox Sensor .....	92
8.5.5	Description of the Calibration of Fluoride Sensors.....	95
8.6	Temperature correction value for pH and fluoride sensors.....	99
<b>9</b>	<b>Measured Variables and Operating Menus for the Standard Signal General.....</b>	<b>101</b>
9.1	Explanation of the Standard Signal General.....	101
9.2	Changing the Measured Variable .....	103
9.3	Reduced / Complete Operating Menu .....	104
9.4	Setting the Reading .....	104
9.5	Description of All Standard Signal Measured Values/Measured Variables .....	105
9.6	Reduced Operating Menu .....	106
9.7	Complete Operating Menu / Description of All Measured Variables .....	108
9.8	Calibrating the Standard Signal .....	109
9.8.1	Calibration of the Zero Point of the Standard Signal General.....	110
9.8.2	Two-Point Calibration of the Standard Signal General.....	111
<b>10</b>	<b>Operating Menus Independent of Measured Variables.....</b>	<b>113</b>
10.1	Pumps .....	114
10.2	Setting the Relays.....	116
10.2.1	Setting and Functional Description of the Relays.....	117
10.3	Setting the Limits.....	122
10.4	Setting the Control.....	125
10.5	Set mA output.....	129
10.6	General settings.....	131
10.6.1	Setting the Measured Variable/Measuring Range.....	131
10.6.2	Sub-Functions of the "General Settings" Menu.....	132
<b>11</b>	<b>Maintenance.....</b>	<b>136</b>
11.1	Fuse replacement DULCOMETER® D1Cb / D1Cc .....	136
11.2	Summary of Error Texts .....	138
<b>12</b>	<b>Technical data.....</b>	<b>141</b>
12.1	Ambient conditions DULCOMETER® D1Cb / D1Cc .....	141
12.2	Sound Pressure Level.....	141
12.3	Material Data.....	142

12.4	Chemical Resistance.....	142
12.5	Dimensions and weights.....	143
<b>13</b>	<b>Electrical Data .....</b>	<b>144</b>
<b>14</b>	<b>Spare parts and accessories DULCOMETER® D1Cb / D1Cc.....</b>	<b>148</b>
<b>15</b>	<b>Standards Complied With .....</b>	<b>150</b>
<b>16</b>	<b>Disposal of Used Parts.....</b>	<b>151</b>
<b>17</b>	<b>Declaration of Conformity.....</b>	<b>152</b>
<b>18</b>	<b>Index.....</b>	<b>154</b>

# 1 Introduction

These operating instructions provide information on the technical data and functions of the DULCOMETER® controllers of the series D1Cb / D1Cc.



*The controllers DULCOMETER® D1Cb and DULCOMETER® D1Cc differ from each other only in their type of housing and mounting location, not in their functionality.*

## 1.1 Explanation of the safety information

### Introduction

These operating instructions provide information on the technical data and functions of the product. These operating instructions provide detailed safety information and are provided as clear step-by-step instructions.

The safety information and notes are categorised according to the following scheme. A number of different symbols are used to denote different situations. The symbols shown here serve only as examples.

### DANGER!

#### **Nature and source of the danger**

Consequence: Fatal or very serious injuries.

Measure to be taken to avoid this danger

Danger!

- Denotes an immediate threatening danger. If this is disregarded, it will result in fatal or very serious injuries.

### WARNING!

#### **Nature and source of the danger**

Possible consequence: Fatal or very serious injuries.

Measure to be taken to avoid this danger

Warning!

- Denotes a possibly hazardous situation. If this is disregarded, it could result in fatal or very serious injuries.





**CAUTION!**

**Nature and source of the danger**

Possible consequence: Slight or minor injuries, material damage.

Measure to be taken to avoid this danger

Caution!

- Denotes a possibly hazardous situation. If this is disregarded, it could result in slight or minor injuries. May also be used as a warning about material damage.



**Type of information**

*Hints on use and additional information*

*Source of the information, additional measures*

*Information!*

- *Denotes hints on use and other useful information. It does not indicate a hazardous or damaging situation.*



**NOTICE!**

**Nature and source of the danger**

Damage to the product or its surroundings

Measure to be taken to avoid this danger

Note!

- Denotes a possibly damaging situation. If this is disregarded, the product or an object in its vicinity could be damaged.

### 1.2 Users' qualifications



#### **WARNING!**

**Danger of injury with inadequately qualified personnel!**

**The operator of the plant / device is responsible for ensuring that the qualifications are fulfilled.**

If inadequately qualified personnel work on the unit or loiter in the hazard zone of the unit, this could result in dangers that could cause serious injuries and material damage.

- All work on the unit should therefore only be conducted by qualified personnel.
- Unqualified personnel should be kept away from the hazard zone

<b>Training</b>	<b>Definition</b>
Instructed personnel	An instructed person is deemed to be a person who has been instructed and, if required, trained in the tasks assigned to him/her and possible dangers that could result from improper behaviour, as well as having been instructed in the required protective equipment and protective measures.
Trained user	A trained user is a person who fulfils the requirements made of an instructed person and who has also received additional training specific to the system from ProMinent or another authorised distribution partner.
Trained qualified personnel	A qualified employee is deemed to be a person who is able to assess the tasks assigned to him and recognize possible hazards based on his/her training, knowledge and experience, as well as knowledge of pertinent regulations. The assessment of a person's technical training can also be based on several years of work in the relevant field.

Training	Definition
Electrician	<p>Electricians are deemed to be people, who are able to complete work on electrical systems and recognize and avoid possible hazards independently based on his/her technical training and experience, as well as knowledge of pertinent standards and regulations.</p> <p>Electricians should be specifically trained for the working environment in which they are employed and know the relevant standards and regulations.</p> <p>Electricians must comply with the provisions of the applicable statutory directives on accident prevention.</p>
Customer Service department	Customer Service department refers to service technicians, who have received proven training and have been authorised by ProMinent to work on the system.



#### *Note for the system operator*

*The pertinent accident prevention regulations, as well as all other generally acknowledged safety regulations, must be adhered to!*

## 1.3 General Safety Information



### **WARNING!**

#### **Live parts!**

Possible consequence: Fatal or very serious injuries

- Measure: Disconnect the mains power supply prior to opening the housing
- De-energise damaged, defective or manipulated units by disconnecting the mains plug



### **WARNING!**

#### **Unauthorised access!**

Possible consequence: Fatal or very serious injuries

- Measure: Ensure that there can be no unauthorised access to the unit

### **WARNING!**

#### **Operating errors!**

Possible consequence: Fatal or very serious injuries

- The unit should only be operated by adequately qualified and technically expert personnel
- Please also observe the operating instructions for controllers and fittings and any other component groups, such as sensors, measuring water pumps ...
- The operator is responsible for ensuring that personnel are qualified

### **CAUTION!**

#### **Electronic malfunctions**

Possible consequence: Material damage to destruction of the unit

- The mains connection cable and data cable should not be laid together with cables that are prone to interference
- Measure: Take appropriate interference suppression measures

### **NOTICE!**

#### **Correct and proper use**

Damage to the product or its surroundings

- The unit is not intended to measure or regulate gaseous or solid media
- The unit may only be used in accordance with the technical details and specifications provided in these operating instructions and in the operating instructions for the individual components

### **NOTICE!**

#### **Correct sensor operation / Run-in time**

Damage to the product or its surroundings

- Correct measuring and dosing is only possible if the sensor is working perfectly
- It is imperative that the run-in times of the sensors are adhered to
- The run-in times should be allowed for when planning initial operation
- It may take a whole working day to run-in the sensor
- Please read the operating instructions for the sensor

**! NOTICE!**

**Correct sensor operation**

Damage to the product or its surroundings

- Correct measuring and dosing is only possible if the sensor is working perfectly
- Check and calibrate the sensor regularly

**! NOTICE!**

**Compensation of control deviations**

Damage to the product or its surroundings

- This controller cannot be used in control circuits which require rapid compensation ( $< 30$  s)

**! NOTICE!**

**Correct and proper use**

The unit is intended to measure and regulate liquid media. The marking of the measured variables is located on the controller and is absolutely binding.

The unit may only be used in accordance with the technical details and specifications provided in this operating manual and in the operating manuals for the individual components (such as, for example, sensors, fittings, calibration devices, metering pumps etc.).

Any other uses or modifications are prohibited.

## 1.4 Correct and proper use

**! NOTICE!**

**Compensation for control deviations**

Damage to the product or its surroundings

- The controller can be used in processes, which require compensation of  $> 30$  seconds

## 1.5 ID Code

### Device identification / Identcode

DULCOMETER® controller series D1Cb / D1Cc			
D1Cb / D1Cc			
<b>Type of mounting</b>			
W	Wall mounted D1Cb (IP 65)		
D	Control panel installation D1Cc (IP54)		
<b>Version</b>			
00	with LCD and keypad / with ProMinent logo		
<b>Operating voltage</b>			
6	90...253 V, 50/60 Hz (wide voltage power unit)		
<b>Certification</b>			
0	CE mark		
1			
<b>Hardware extension I</b>			
0	none		
<b>Hardware extension II</b>			
0	none		
1	Protective RC circuit for power relay		
<b>External connection</b>			
0	none		
<b>Software default setting</b>			
U	Default setting		
V	Software preset		
<b>Default measured variable</b>			
0	Universal	I	Chlorite
A	Peracetic acid	P	pH

## DULCOMETER® controller series D1Cb / D1Cc

B	Bromine	R	ORP
C	Chlorine	S	0/4...20 mA standard signal general
D	Chlorine dioxide	X	Dissolved oxygen
F	Fluoride	Z	Ozone
H	Hydrogen peroxide	L	Conductivity

**Connection of the measured variable**

1	mA input (standard signal 0/4-20 mA, all measured variables)
---	--

5	mV input (pH/ORP)
---	-------------------

**Correction variable**

0	none
---	------

2	Temperature Pt 100/PT1000 (for pH, conductivity, fluoride, ClO <sub>2</sub> CDP sensor)
---	---

4	Manual temperature input (for pH, conductivity, fluoride, ClO <sub>2</sub> CDP sensor)
---	--

**Control input**

0	none
---	------

1	Pause
---	-------

**Signal output**

0	none
---	------

1	Analogue signal output 0/4...20 mA
---	------------------------------------

**Power activation**

G	Alarm and 2 limit relays
---	--------------------------

**DULCOMETER® controller series D1Cb / D1Cc**

	M	Alarm and 2 solenoid valve relays		
		<b>Pump activation</b>		
	0	none		
	2	2 pumps via pulse frequency		
		<b>Control characteristic</b>		
		0	none	
		1	Proportional control	
		2	PID control	



## 2 Functional description

### Brief functional description

The DULCOMETER® D1Cb / D1Cc 4-wire measuring transducer/controller is a device designed to measure/control a measured variable.

In the mA measuring version, the measured variable can be changed without restrictions in the device menu. In the mV measurement version, the menu of the DULCOMETER® D1Cb / D1Cc only permits choice between pH and ORP.

Depending on the measured variable, sensors for pH or redox potential (ORP) or amperometric sensors can only be connected to the measured variables in line with *Allocation of the measurement inputs of the DULCOMETER® D1Cb / D1Cc' Table on page 17*. The temperature measurement serves as a correction variable and can be measured using a Pt 100/1000. This means that automatic temperature compensation is possible with pH-value, conductivity and fluoride measured variables. Temperature compensation is performed in the sensor (with the exception of the chlorine dioxide sensor type CDP) with amperometric measured variables (chlorine etc.). Operation of the DULCOMETER® D1Cb / D1Cc takes place via the menu keys. and the data is displayed by means of an illuminated LCD display. The LCD display ensures that the measured value, correction variable, control value and error messages can be clearly read.

### Allocation of the measurement inputs of the DULCOMETER® D1Cb / D1Cc

		Connection of the measured variable to:	
Character	Measured variable	mV input	mA input
0	no default setting of the measured variable (pH and redox can be selected)	X	
A	PES (peracetic acid)		X
B	Bromine		X
C	Chlorine		X
D	Chlorine dioxide		X
F	Fluoride		X
*with measured value transducer			

## Functional description

		Connection of the measured variable to:	
Character	Measured variable	mV input	mA input
H	H <sub>2</sub> O <sub>2</sub> (hydrogen peroxide)		X
I	Chlorite		X
P	pH	X	X*
R	ORP	X	X*
S	0/4...20 mA standard signal general		X
X	O <sub>2</sub>		X
Z	O <sub>3</sub>		X
L	Conductivity		X
<b>*with measured value transducer</b>			

Description of the terminal connections for mA and mV: see Fig. 11 and Fig. 12

Description of the operating menu of the measured variables via mV connection: see [Chapter 8 'Measured Variables and Operating Menus for Potentiometric Sensors'](#) on page 81

Description of the operating menu of the measured variables via mA connection: see [Chapter 7 'Measured Variables and Operating Menus for Amperometric Sensors'](#) on page 69

Description of the operating menu of the measured variables via mA standard signal: see [Chapter 9 'Measured Variables and Operating Menus for the Standard Signal General'](#) on page 101

### 2.1 Wall mounting/control panel installation

#### DULCOMETER® D1Cb

The DULCOMETER® D1Cb W is suitable both for wall-mounting, as well as for installation in a control panel (with additional control panel mounting kit).

The plastic housing comprises a housing upper section and lower section. The LCD display and membrane keypad are accommodated in the upper section of the housing.

The lower section of the housing accommodates the processor and power units and any optional assemblies. A ribbon cable connects to the LCD display and the membrane keypad.

The electrical connection is made through originally sealed, push-out cable cut-outs on the underside of the lower section of the housing.

A wall bracket for wall mounting is located on the rear of the lower section of the housing.

### **DULCOMETER® D1Cc**

The DULCOMETER® D1Cc is suitable for control panel installation. In this respect it fulfils the same functions as the D1Cb. However, the D1Cc also has an option for upgrading with a protective RC circuit. When correctly installed, the D1Cc has an IP54 protection rating.

## **2.2 Electrical construction**

The device does not have a mains switch. It is therefore immediately ready for operation once connected to the power supply.

The device processes an input signal whilst taking into consideration operator inputs. The result is displayed and made available to other devices via a standard signal. When equipped with actuators, the device can also provide control functions. It is designed to activate metering pumps, solenoid valves, as well as an mA standard signal output. The activation variable is recalculated every second.

## 2.2.1 Block circuit diagram

### ! NOTICE!

#### Connection of mV or mA sensors

The DULCOMETER® D1Cb / D1Cc is suitable for the connection of mV or mA sensors. It is not possible to connect mV and mA sensors simultaneously.

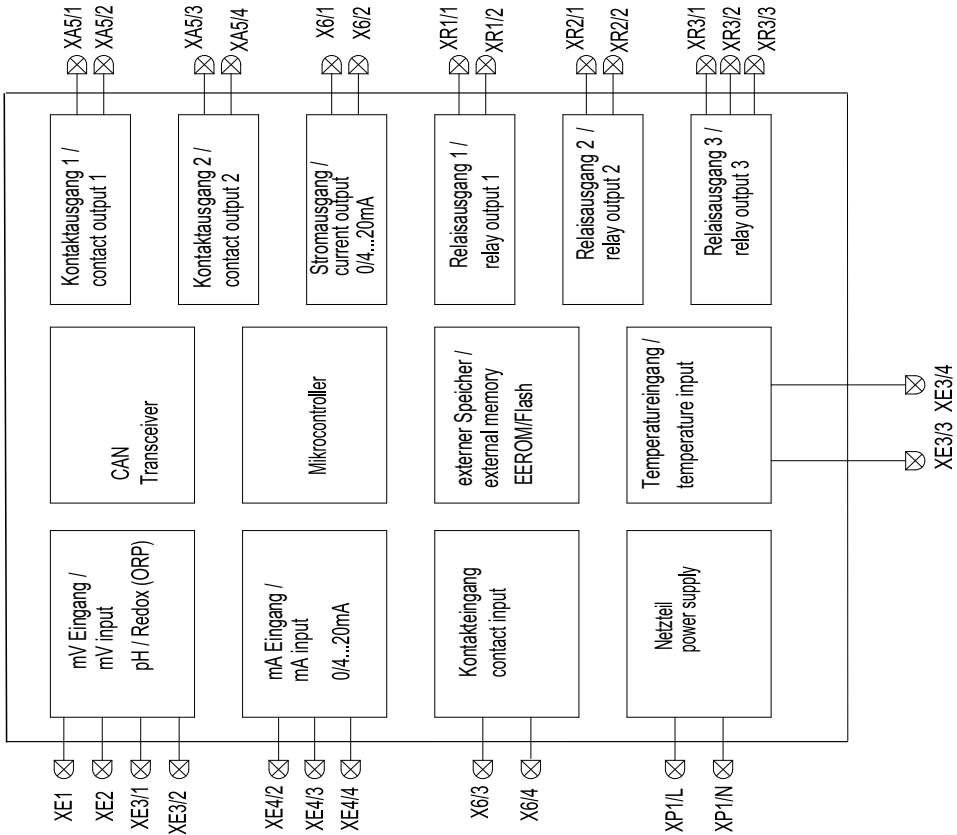


Fig. 1: Block circuit diagram

## 2.2.2 Galvanic Isolation



### WARNING!

#### Protective low voltage/Mains voltage

Possible consequence: Fatal or very serious injuries

If relay 1 or 2 is operated with protective low voltage, no mains voltage may be connected to the other relay.

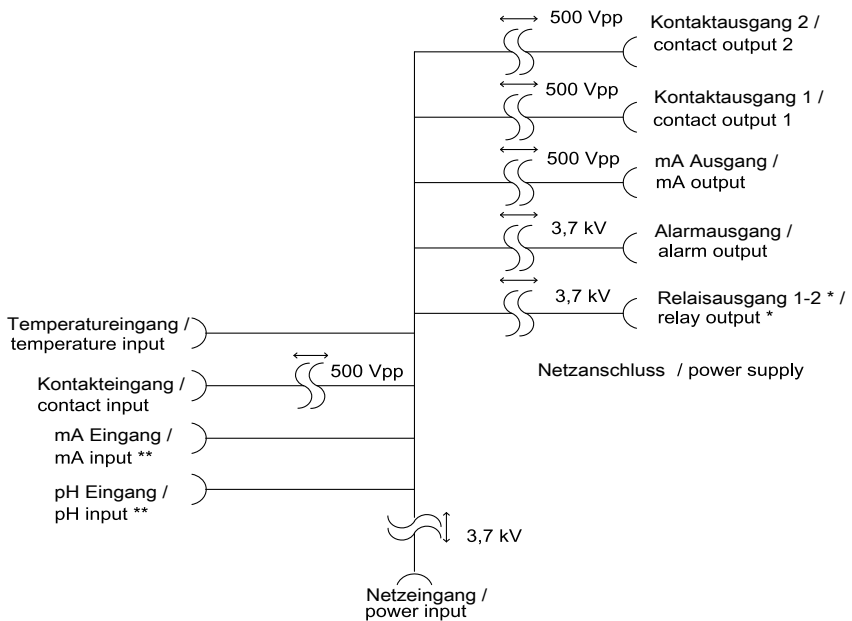




Fig. 2: Galvanic Isolation

\* If relay 1 or 2 is operated with protective low voltage, no mains voltage may be connected to the other relay.

\*\* No galvanic isolation between mA and mV input and temperature input.

### 3 D1Cb mounting

- **User qualification, mechanical mounting:** trained qualified personnel, see  *Chapter 1.2 'Users' qualifications' on page 10*
- **User qualification, electrical installation:** Electrical technician, see  *Chapter 1.2 'Users' qualifications' on page 10*

#### NOTICE!

##### Mounting position and conditions

- Ensure that there is unimpeded access for operation
- Secure, low-vibration fixing
- Avoid direct sunlight
- Permissible ambient temperature at fixing position: 0 ... 50 °C at max. 95 % relative air humidity (non-condensing)

#### NOTICE!

##### Material damage to electrostatically sensitive components

Components can be damaged or destroyed by electrostatic voltages.

- Before any work, on electrostatically sensitive components, disconnect the power supply.
- When working on electrostatically sensitive components, wear an earthed anti-static wrist band.
- Always hold components by their corners and never touch conductors, ICs, etc.
- Only place components on anti-static supports or the original packaging.



##### *Ablese- und Bedienposition*

- *Das Gerät in einer günstigen Ablese- und Bedienposition (möglichst in Augenhöhe) montieren*



##### *Montageposition*

- *Ausreichend Freiraum für die Kabel vorsehen*
- *Für die 'Parkstellung' des Reglers, nach oben mindestens 120 mm Platz freihalten*

### 3.1 Scope of supply

The following parts belong to the standard scope of supply of a DULCOMETER® series D1Cb controller.

Identifier	Quantity
D1Cb controller	1
Half screw connection, complete (set)	1
M12 x 1.5 threaded connection, complete (set)	1
Assembly material, complete, 3P Universal (set)	1
Measured variable labels D1C/D2C	1
Operating Manual	1
General safety notes	1

### 3.2 Installation (Wall Mounted)

The device can be installed directly on the wall with the aid of the wall bracket.

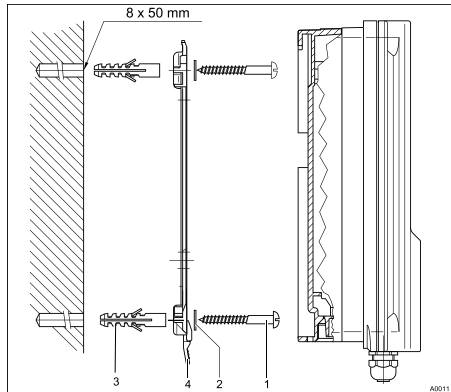


Fig. 3: Fixing material for wall mounting

- |                               |                    |
|-------------------------------|--------------------|
| 1. 3 x Round head screws 5x45 | 2. 3 x Washers 5.3 |
| 3. 3 x Plastic wall plugs d8  | 4. Wall bracket    |
1. ➤ Mark the holes using the wall bracket and drill them
  2. ➤ Insert wall plugs
  3. ➤ Secure wall bracket in place with washers and round head screws
  4. ➤ Place the device from above onto the wall bracket
  5. ➤ Press the device gently against the wall bracket and slide it approx. 4 mm upwards until you hear it engage in position



### 3.3 Installation - Control Panel Mounted (Optional)

#### CAUTION!

##### Dimensional variations

Possible consequence: material damage

- Photocopying the punched template can result in dimensional deviations
- Use the dimensions shown in Fig. 4 and mark on the control panel

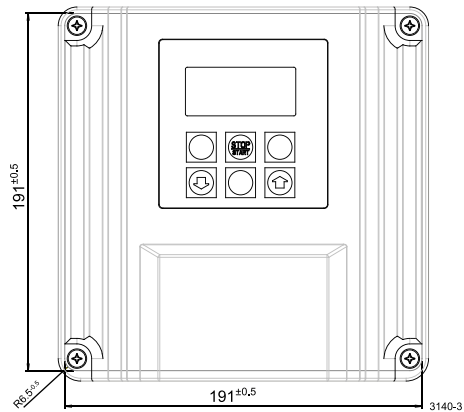



Fig. 4: Punched template, drawing number 3140-3 /not to scale

#### CAUTION!

##### Material thickness of control panel

Possible consequence: material damage

- The material thickness of the control panel must be at least 2 mm to ensure secure fixing

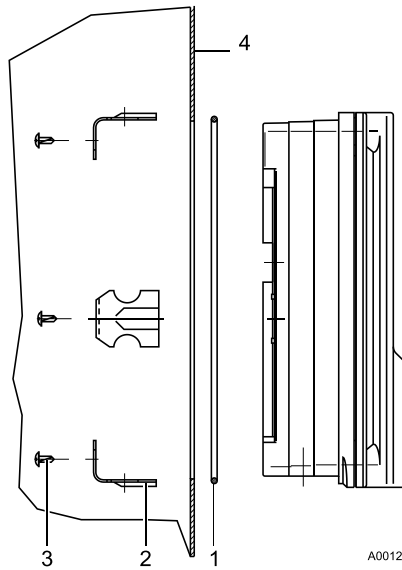


*Fig. 5: The material thickness of the control panel must be at least 2 mm to ensure secure fixing*







1. 1 x Foam rubber caulk strip d3

2. 6 x Galvanised steel retaining brackets

3. 6 x Galvanised PT cutting screws

4. Control panel

For the part number of the assembly set, refer to  *Table on page 149*

1.  Using the dimensions shown in Fig. 4 mark the precise position of the device on the control panel
2.  Mark the corner points and drill (drill diameter 12 - 13 mm)
3.  With a punching tool or jigsaw make the opening as per the punched template drawing
4.  Chamfer the cut edges and check whether the sealing surfaces are smooth for the caulk strip
  - ⇒ Otherwise the seal cannot be guaranteed
5.  Press the caulk strip evenly into the groove running around the device
6.  Place the device into the control panel and fix in place at the rear by means of the retaining brackets and PT cutting screws
  - ⇒ The device should project approx. 35 mm from the control panel

### 3.4 Wall Mounted Installation of D1Cb (Electrical)



#### **WARNING!**

#### **Electrical voltage**

Possible consequence: Fatal or very serious injuries

- The electrical connection to the device should only be made once it has been fitted to the wall or control panel
- The device must be electrically disconnected before it is opened
- Ensure that the device cannot be reconnected accidentally

#### **! NOTICE!**

#### **Opening the device**

Damage to the product or its surroundings

- The device may only be opened by qualified personnel
- The device should only be opened when fitted to the wall or control panel

### 3.4.1 Opening the device

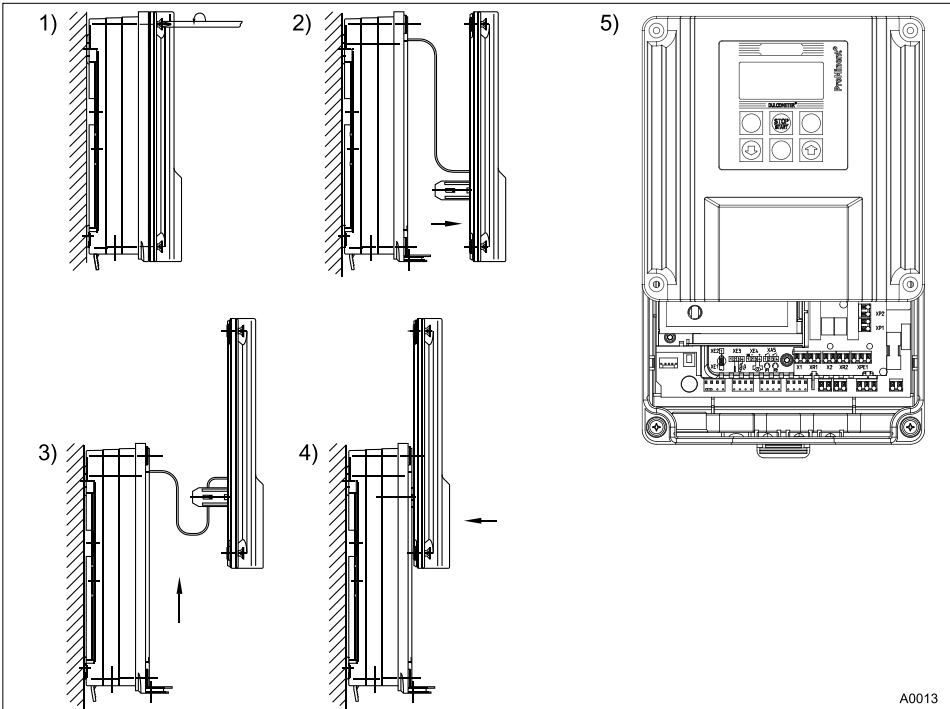


Fig. 6: Opening the device

1. ➤ Loosen the 4 captive screws (1).
2. ➤ Lift the upper section of the device from the lower section (2). A wide flathead screwdriver may be of assistance.
3. ➤ Insert the upper section with both guide rails into the lower section (3 and 4) (parked position)

### 3.4.2 Electrical Installation (Wall Mounted)

**! NOTICE!**

**Threaded holes**

Using a suitable tool, punch out the threaded holes according to the number of cables (  $\varnothing$  approx. 4 mm).

- Punch aids are provided to punch out the threaded holes

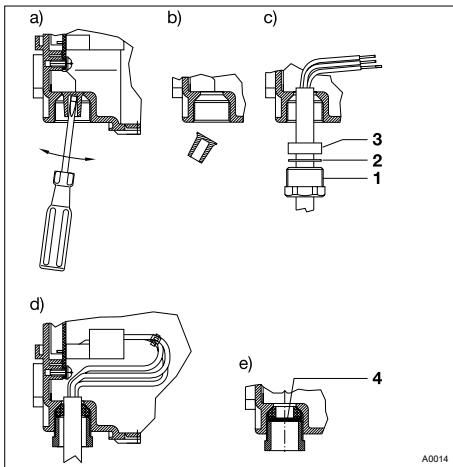


Fig. 7: Punching out the threaded holes

1. Screw connection M20 x 1.5	2. Pressure ring M20
3. Pressure ring M20	4. Dummy washer M20

1. ➤ Remove cable sheathing over a sufficient length
2. ➤ Fit screw connection (1), pressure ring (2) and seal (3) onto cable
3. ➤ Insert cable and fittings into the threaded hole
4. ➤ Align the cable and push in until enough cable is in the control housing
5. ➤ Screw in screw connection and tighten firmly
6. ➤ Shorten cable wires to the precise overall length and strip off approx. 8 mm insulation
7. ➤ Fit cable end sleeves to the wires. Refer to on page 32
8. ➤ Connect up the wires to the terminals according to the electrical wiring diagram Fig. 11

Punched out threaded holes can be resealed with the M20 dummy washers (4) provided.

The M12 x 1.5 screw connections and brass lock nuts are used for the 4 openings in the front row.

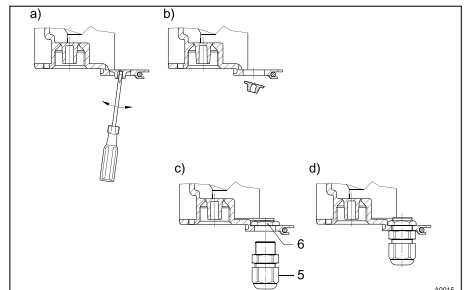


Fig. 8: M12x1.5 screw connections

5. Screw connection M12 x 1.5

6. Lock nut M12x1.5

1. ➤ Fit lock nut M12x1.5 (6) on the inside
2. ➤ Fit screw connection M12x1.5 (5) from the outside and tighten firmly

### 3.4.3 Electrical Installation (Control Panel Mounted)

Proceed as described under "Electrical Installation (Wall Mounted)". Refer to [Chapter 3.4.2 'Electrical Installation \(Wall Mounted\)'](#) on page 29

Only the rear row of threaded holes (M20x1.5) should be used when the device is mounted in a control panel. The front row (M12x1.5) lies outside of the control panel.

Connect up as per the electrical terminal wiring diagram. Refer to [Chapter 3.4.7 'Terminal Wiring Diagram'](#) on page 34

### 3.4.4 Installation of Coaxial Cable to Guard Terminal XE1



#### CAUTION!

##### Maximum length of the coaxial cable 10 m

Incorrect reading due to too long a coaxial cable

Possible consequence: Slight or minor injuries, material damage

The maximum length of the coaxial cable may not exceed 10 m when using redox or pH sensors. The measured signal can otherwise be falsified by the effects of interference.


If the gap between the pH/redox measuring point and the DULCOMETER® D1Cb is more than 10 metres, then the use of an interposed DULCOTEST® transducer 4-20 mA pH V1, rH V1 is recommended. The connection is then made via terminal XE4 of the DULCOMETER® D1Cb.

The XE4 (mA input) terminal is a chargeable additional function!

When installing the coaxial cable for the guard terminal XE 1, the allowances shown on the diagram for stripping insulation from the coaxial cable should be adhered to. Fig. 9

The guard terminal should be tightened until "hand-tight".

# D1Cb mounting

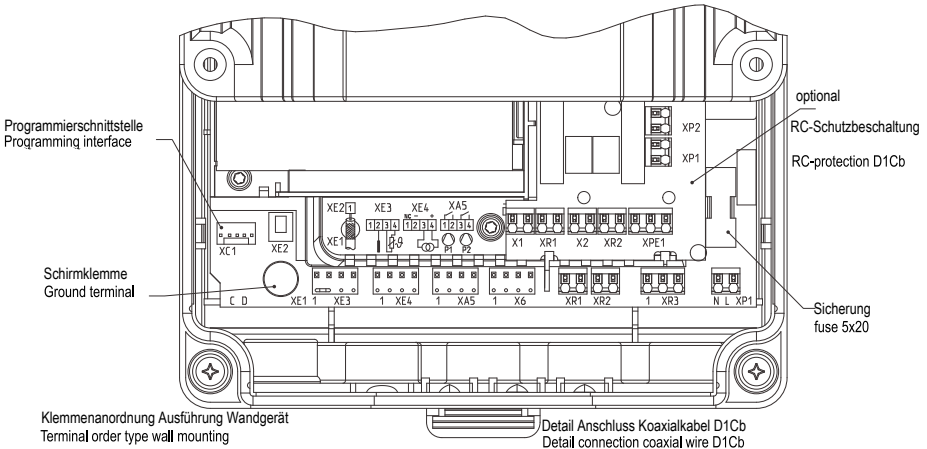

Manufacturing coaxial cable for the connection at D1Cb  
 or prefabricates in the variants  
 Konfektionierung Koaxialkabel zum Anschluss an D1Cb  
 oder vorkonfektioniert in den Varianten





Fig. 9: Preparation of coaxial cable

## 3.4.5 Cable Cross-Sections and Cable End Sleeves

	Minimum cross-section	Maximum cross-section	Stripped insulation length
Without cable end sleeve	0.25 mm <sup>2</sup>	1.5 mm <sup>2</sup>	
Cable end sleeve without insulation	0.20 mm <sup>2</sup>	1.0 mm <sup>2</sup>	8 - 9 mm
Cable end sleeve with insulation	0.20 mm <sup>2</sup>	1.0 mm <sup>2</sup>	10 - 11 mm

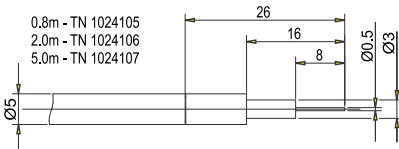

### **3.4.6 Protective RC Circuit (Optional)**

A protective RC circuit is recommended for operation with consumers, which present an inductive load (e.g. motor metering pumps or solenoid metering pumps). In these applications a protective RC circuit prevents wear and tear of the relay contacts. Refer to ↪ *'Spare parts and accessories DULCOMETER® D1Cb'* on page 148

3.4.7 Terminal Wiring Diagram

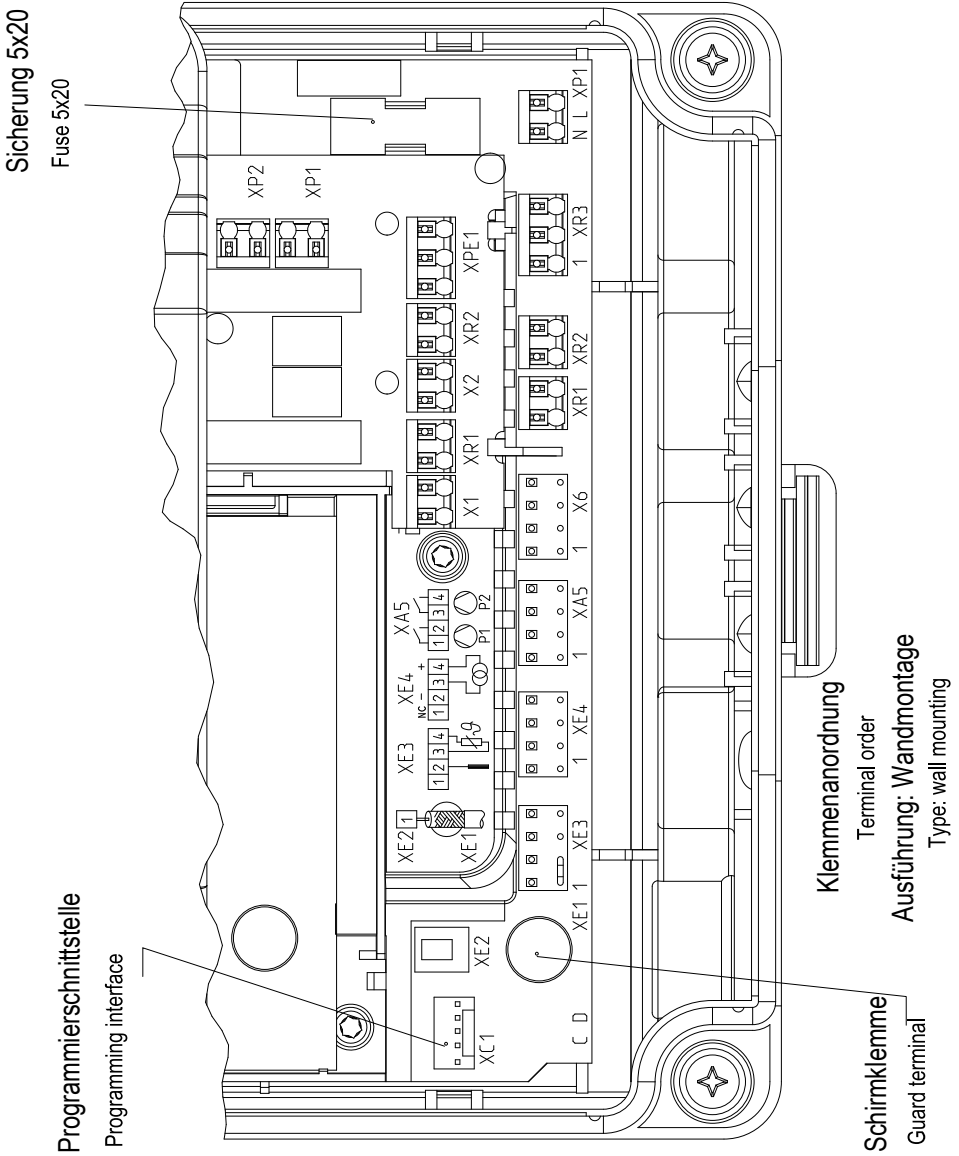


Fig. 10: Terminal layout

# Belegungsvarianten

(ohne RC-Schutzbeschaltung)  
**Assignment variants**  
 (without Protective RC Circuit)

Variant 1	Magnetventil
variant 1	solenoid valve
Variant 2	Grenzwertrelais, Timer, Stellglied
variant 2	limit relay, timer, actuator

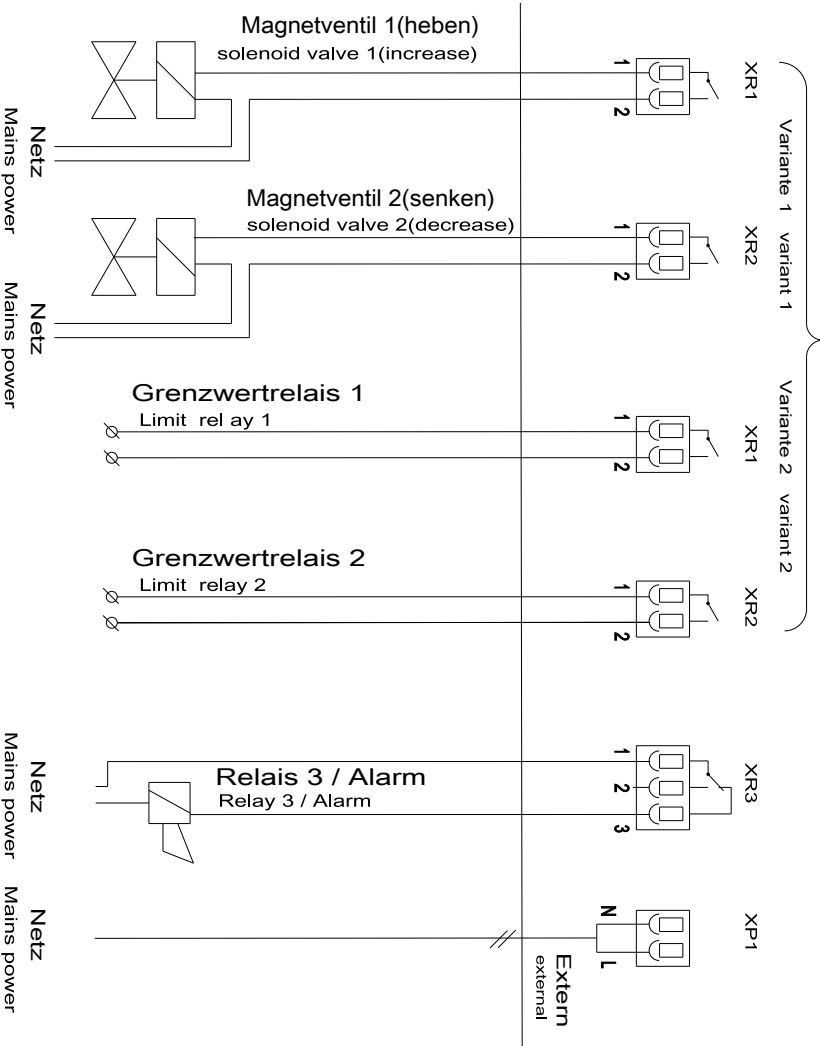


Fig. 11: Terminal diagram with assignment options 1

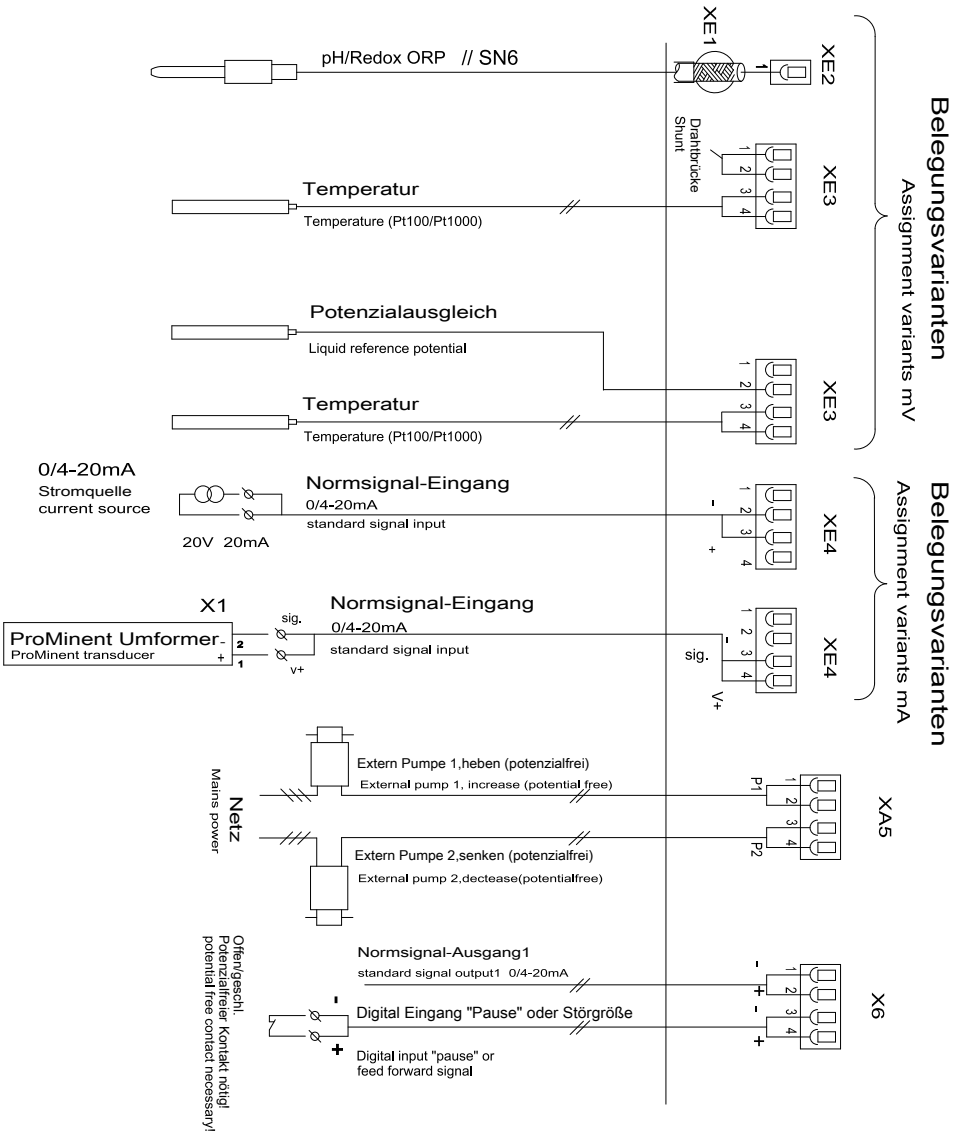


Fig. 12: Terminal diagram with assignment options 2

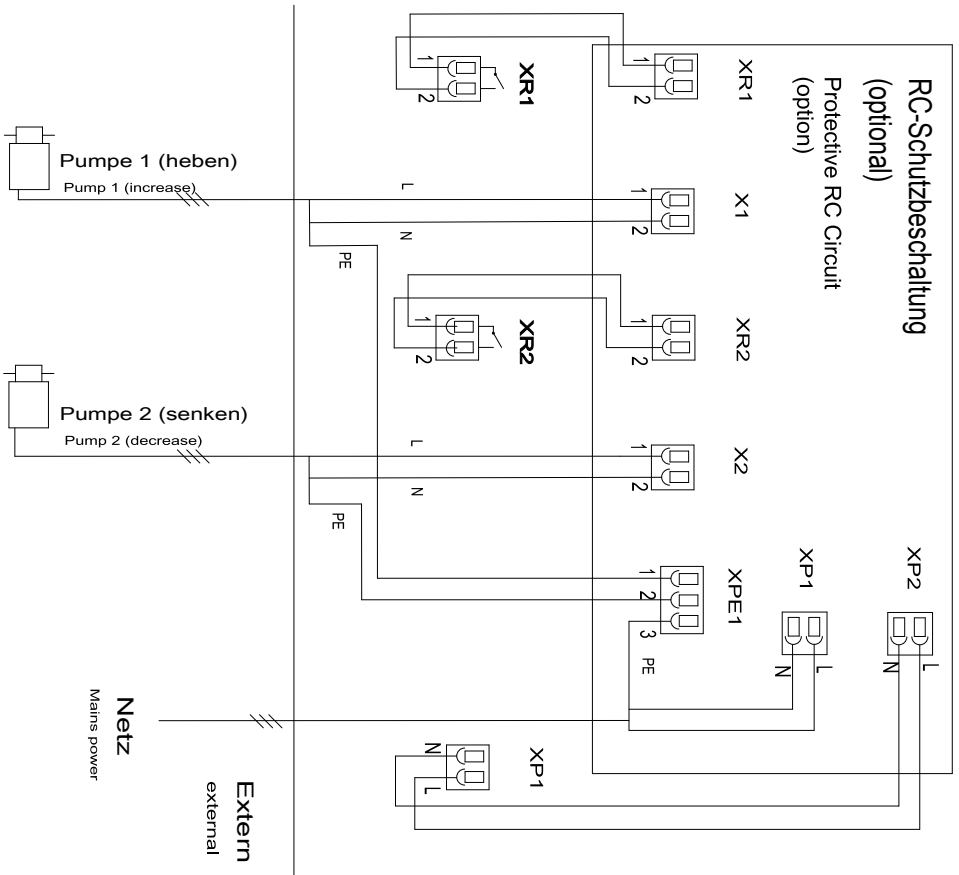


Fig. 13: Protective RC circuit terminal diagram

### 3.5 Switching of inductive loads



*If you connect an inductive load, i.e. a consumer which uses a coil (e.g. an alpha motorised pump), then you must protect your controller with a protective circuit. If in doubt, consult an electrical technician for advice.*

The RC member protective circuit is a simple, but nevertheless very effective, circuit. This circuit is also referred to as a snubber or Boucherot member. It is primarily used to protect switching contacts.

When switching off, the connection in series of a resistor and capacitor means that the current can fade out in a damped oscillation.

Also when switching on, the resistor acts as a current limiter for the capacitor charging process. The RC member protective circuit is highly suited to AC voltage supplies.

The magnitude of the resistance R of the RC member is determined according to the following equation:

$$R=U/I_L$$

(U= Voltage divided by the load //  $I_L$  = load current)

The magnitude of the capacitor is determined using the following equation:

**Units: R = Ohm; U = Volt;  $I_L$  = Ampere; C =  $\mu$ F**

$$C=k * I_L$$

$k=0,1...2$  (dependent on the application).


Only use capacitors of class X2.

**Units: R = Ohm; U = Volt;  $I_L$  = Ampere; C =  $\mu$ F**



*If consumers are connected which have a high starting current (e.g. plug-in, switched mains power supplies), then a means of limiting the starting current must be provided.*

The switching-off process can be investigated and documented using an oscilloscope. The voltage peak at the switch contact depends on the selected RC combination.

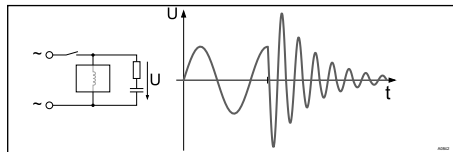


*Fig. 14: Switching-off process shown on the oscillogram.*

**WARNING!****Mains voltage**

Possible consequence: Fatal or very serious injuries

If mains voltage is connected to one of the terminals XR1-XR3 or XP, then no protective low voltage may be connected to any other of these terminals (SELV).

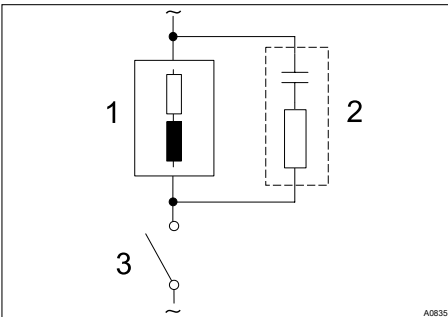

*Fig. 15: RC protective circuit for the relay contacts*

Typical AC current application with an inductive load:

- 1) Load (e.g. alpha motorised pump)
- 2) RC-protective circuit
  - Typical RC protective circuit at 230 V AC:
  - Capacitor  $[0.22\mu F/X2]$
  - Resistor  $[100\text{ ohm} / 1\text{ W}]$  (Metal-oxide (pulse-resistant))
- 3) Relay contact (XR1, XR2, XR3)

### 4 D1Cc mounting

- **User qualification, mechanical mounting:** trained qualified personnel, see ↗ *Chapter 1.2 'Users' qualifications' on page 10*
- **User qualification, electrical installation:** Electrical technician, see ↗ *Chapter 1.2 'Users' qualifications' on page 10*

#### ! NOTICE!

##### Mounting position and conditions

- Ensure that there is unimpeded access for operation
- Secure, low-vibration fixing
- Avoid direct sunlight
- Permissible ambient temperature at fixing position: 0 ... 50 °C at max. 95 % relative air humidity (non-condensing)

#### ! NOTICE!

##### Material damage to electrostatically sensitive components

Components can be damaged or destroyed by electrostatic voltages.

- Before any work, on electrostatically sensitive components, disconnect the power supply.
- When working on electrostatically sensitive components, wear an earthed anti-static wrist band.
- Always hold components by their corners and never touch conductors, ICs, etc.
- Only place components on anti-static supports or the original packaging.



##### *Ablese- und Bedienposition*

- *Das Gerät in einer günstigen Ablese- und Bedienposition (möglichst in Augenhöhe) montieren*



##### *Montageposition*

- *Ausreichend Freiraum für die Kabel vorsehen*



## 4.1 DULCOMETER® D1Cc scope of supply

The following parts belong to the standard scope of supply of a DULCOMETER® series D1Cc controller.

Identifier	Quantity
D1Cc controller	1
Retaining bracket	4
Measured variable labels D1C/D2C	1
Operating Manual	1
General safety notes	1

## 4.2 Mounting - control panel installation DULCOMETER® D1Cc



### CAUTION!

#### Dimensional variations

Possible consequence: material damage

- Photocopying the punched template can result in dimensional deviations
- Use the dimensions according to Fig. 16 and mark on the control panel



### CAUTION!

#### Material thickness of control panel

Possible consequence: material damage

- The material thickness of the control panel must be at least 2 mm to ensure secure fixing

The device is designed for installation in a control panel. The housing corresponds to DIN 43700. The control panel opening for installation of the device is specified in DIN 43700. We recommend a smaller opening. Fixing of the device is then better (less sideways play) and the seal is uniformly compressed.

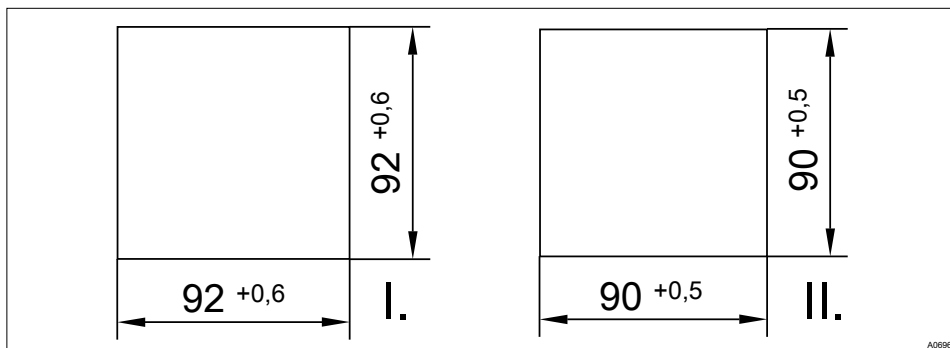


Fig. 16: Mounting - control panel installation DULCOMETER® D1Cc

- I. DIN 43700 instruction
- II. ProMinent recommendation

### Fabricating the opening:

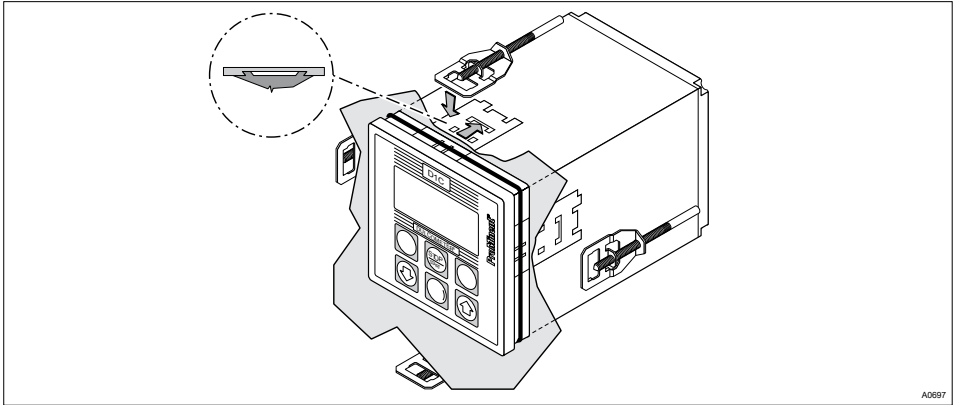


Fig. 17: Screw the studs forward



*A drilling punched 1:1 template is enclosed with the device as a mounting aid. Its use will ensure optimal positioning of the device on the control panel.*


1. ➤ Align and secured the punched drilling template in the appropriate position on the control panel using a spirit level
2. ➤ Mark the four corners using a centre punch and drill four holes using a 6 mm Ø bit
3. ➤ Then saw out the connected bridges with a jigsaw
4. ➤ Dress the surfaces so they are smooth and the dimensions are within the specified tolerance.
5. ➤ Finally ensure the edges are fully de-burred
6. ➤ Before inserting the device in the control panel opening, check the position of the seal (must lie against the front collar)



*IP54 protection rating*

7. ➔ Insert the device from the outside in the opening, attach the retaining bracket and push backwards up to the stop
  - ⇒ All four holes retaining brackets must be attached, as otherwise protection rating IP54 cannot be adhered to.
8. ➔ Using a suitable screw driver, screw the studs forwards, see Fig. 17, until the seal is completely and uniformly compressed
9. ➔ Check the correct seating of the seal, as necessary loosen the studs and correct the position

### 4.3 Electrical Installation (Control Panel Mounted)

Connect up as per the electrical terminal wiring diagram. Refer to  *Chapter 4.3.3 'Terminal diagram' on page 48*

### 4.3.1 Installation of Coaxial Cable to Guard Terminal XE1



#### **CAUTION!**

##### **Maximum length of the coaxial cable 10 m**

Incorrect measured value due to too long a coaxial cable

Possible consequence: Slight or minor injuries. Material damage.

The maximum length of the coaxial cable may not exceed 10 m when using redox or pH sensors. The measurement signal can otherwise be falsified by the effects of interference.


If the distance between the pH/ORP measuring point and the DULCOMETER® D1Cc is more than 10 m, the use of a DULCOTEST® measuring transducer 4-20 mA pH V1, rH V1 is recommended. Connection is then via terminal XE4 of the DULCOMETER® D1Cc

The XE4 (mA input) terminal is an auxiliary function that incurs an extra charge.

When installing the coaxial cable for the guard terminal XE 1, the allowances shown in the diagram Fig. 18 for stripping insulation from the coaxial cable must be adhered to. The guard terminal should be tightened until "hand-tight".

## D1Cc mounting

Terminal order panel type mounting  
Terminal order type panel mounting

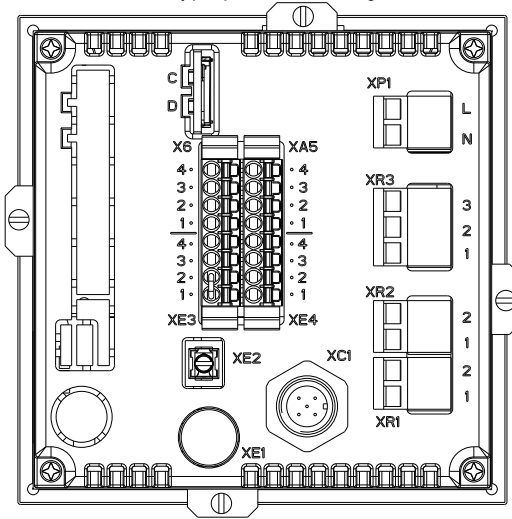

Manufacturing coaxial cable for the connection at D1Cc  
or prefabricates in the variants

Fabrication of the coaxial cable connection to the D1Cc  
or pre-fabricated for the variants

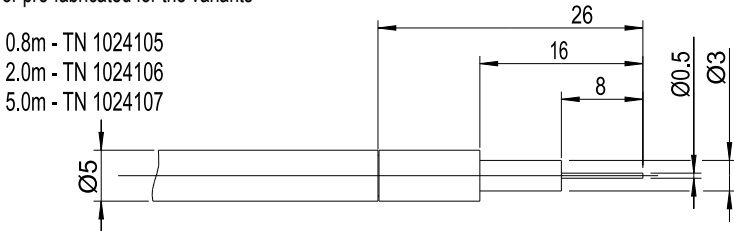


Fig. 18: Preparation of coaxial cable

### 4.3.2 Cable Cross-Sections and Cable End Sleeves

	Minimum cross-section	Maximum cross-section	Stripped insulation length
Without cable end sleeve	0.25 mm <sup>2</sup>	1.5 mm <sup>2</sup>	
Cable end sleeve without insulation	0.20 mm <sup>2</sup>	1.0 mm <sup>2</sup>	8 - 9 mm
Cable end sleeve with insulation	0.20 mm <sup>2</sup>	1.0 mm <sup>2</sup>	10 - 11 mm

### 4.3.3 Terminal diagram

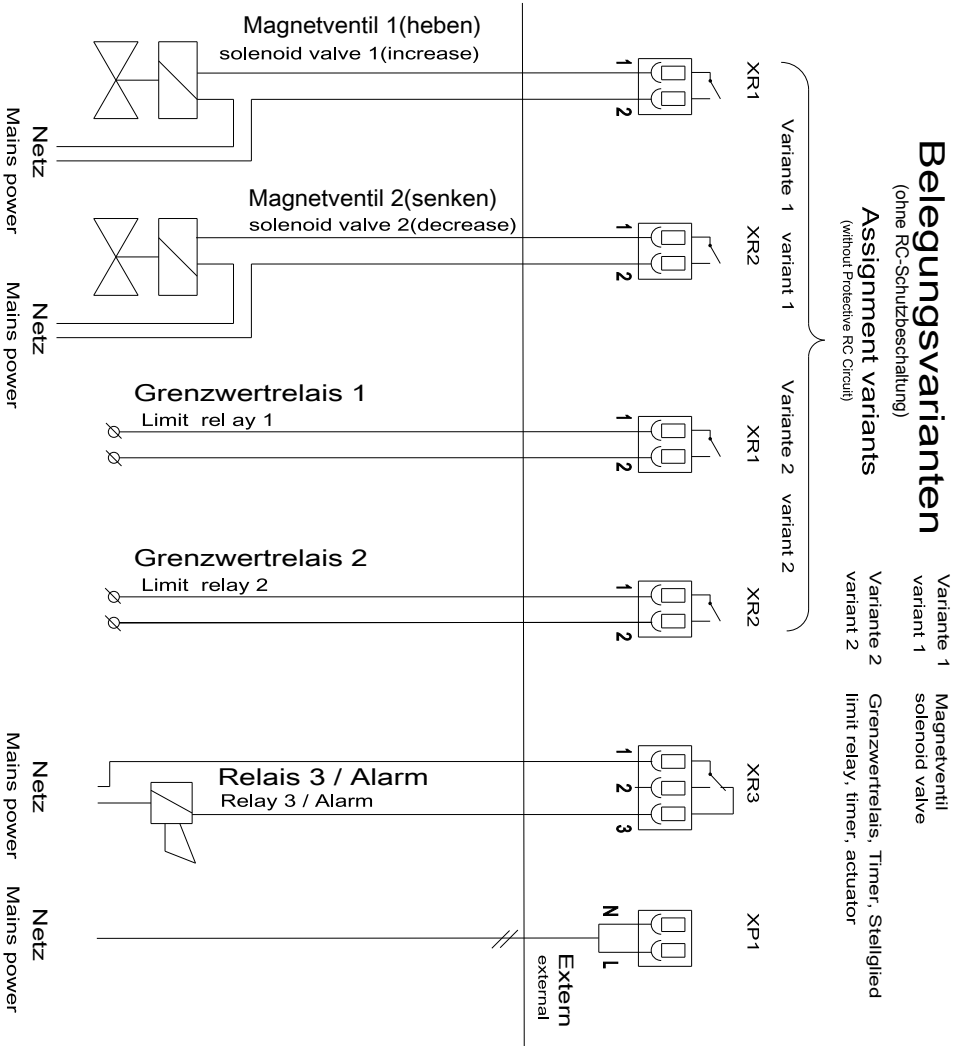


Fig. 19: Terminal diagram with assignment options 1



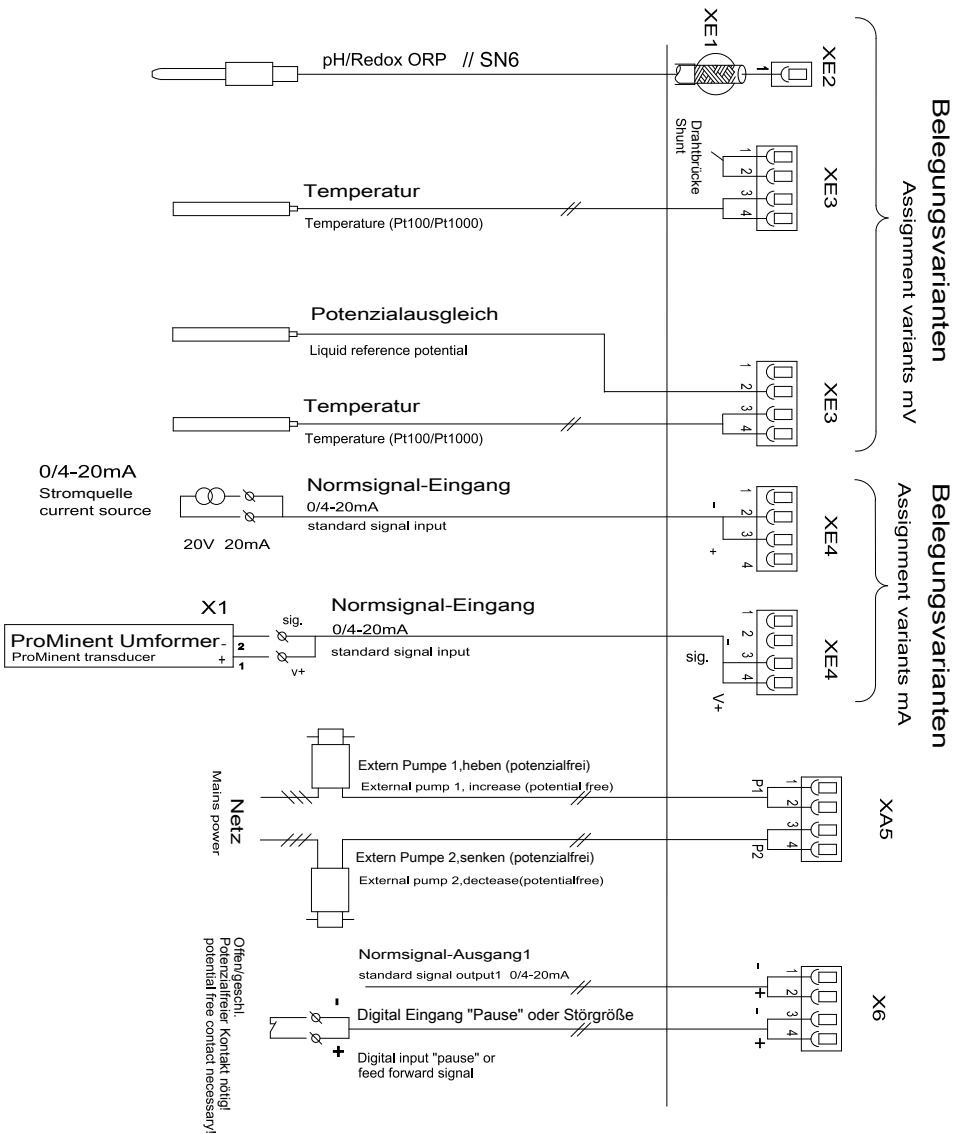


Fig. 20: Terminal diagram with assignment options 2

### 4.4 Switching of inductive loads



*If you connect an inductive load, i.e. a consumer which uses a coil (e.g. an alpha motorised pump), then you must protect your controller with a protective circuit. If in doubt, consult an electrical technician for advice.*

The RC member protective circuit is a simple, but nevertheless very effective, circuit. This circuit is also referred to as a snubber or Boucherot member. It is primarily used to protect switching contacts.

When switching off, the connection in series of a resistor and capacitor means that the current can fade out in a damped oscillation.

Also when switching on, the resistor acts as a current limiter for the capacitor charging process. The RC member protective circuit is highly suited to AC voltage supplies.

The magnitude of the resistance R of the RC member is determined according to the following equation:

$$R=U/I_L$$

(U= Voltage divided by the load //  $I_L$  = load current)

The magnitude of the capacitor is determined using the following equation:

$$\text{Units: } R = \text{Ohm}; U = \text{Volt}; I_L = \text{Ampere}; C = \mu\text{F}$$

$$C=k * I_L$$

$k=0,1...2$  (dependent on the application).


Only use capacitors of class X2.

$$\text{Units: } R = \text{Ohm}; U = \text{Volt}; I_L = \text{Ampere}; C = \mu\text{F}$$



*If consumers are connected which have a high starting current (e.g. plug-in, switched mains power supplies), then a means of limiting the starting current must be provided.*

The switching-off process can be investigated and documented using an oscilloscope. The voltage peak at the switch contact depends on the selected RC combination.

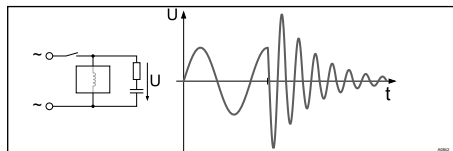


*Fig. 21: Switching-off process shown on the oscillogram.*

**WARNING!****Mains voltage**

Possible consequence: Fatal or very serious injuries

If mains voltage is connected to one of the terminals XR1-XR3 or XP, then no protective low voltage may be connected to any other of these terminals (SELV).

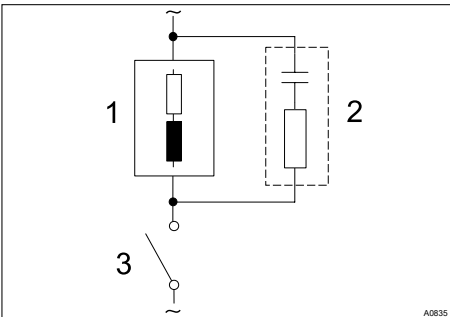

*Fig. 22: RC protective circuit for the relay contacts*

Typical AC current application with an inductive load:

- 1) Load (e.g. alpha motorised pump)
- 2) RC-protective circuit
  - Typical RC protective circuit at 230 V AC:
  - Capacitor  $[0.22\mu F/X2]$
  - Resistor  $[100\text{ ohm} / 1\text{ W}]$  (Metal-oxide (pulse-resistant))
- 3) Relay contact (XR1, XR2, XR3)

## 5 Commissioning

- **Users' qualification:** Trained user

### **WARNING!**

#### **Sensor run-in periods**

This can result in hazardous incorrect metering

Take into consideration run in periods when commissioning

- Correct measuring and dosing is only possible if the sensor is working perfectly
- It is imperative that the run in periods of the sensors are adhered to
- The run in periods should be allowed for when planning commissioning
- It may take a whole working day to run-in the sensor
- Please read the operating manual for the sensor

Following completion of mechanical and electrical assembly, the controller should be integrated into the measuring point.


### 5.1 Initial commissioning

During initial commissioning the device's display will be in "English". The display will show "language english". Exception: the language has been factory-preset to the customer's requirement.

### **Start menu during initial commissioning**

*The "Language setting during initial commissioning" menu appears only once.*

*Later changes to the operating language can then be made via the "General Settings/Information" menu item.*

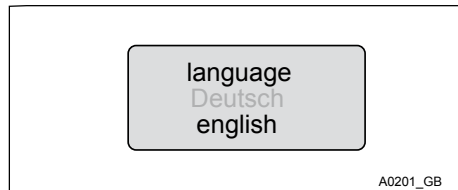

*Fig. 23: Initial commissioning display*




This is followed by the selection of the measured variable and the measuring range in the "General Settings/Information" menu item.


#### 5.1.1 Selection of the Operating Language

With devices, which have not been pre-configured to the customer's specific requirement, the operating language required has to be selected in the "General Settings / Operating Menu" menu. Refer to [Chapter 10.6 'General settings'](#) on page 131

**! NOTICE!****Resetting the operating language**

In the event that a foreign and thus non-comprehensible operating language has been set, the DULCOMETER® D1Cb / D1Cc can be reset to the basic "English" setting.

If you find yourself in the continuous display 1, then by simultaneously pressing the keys , ,  the DULCOMETER® D1Cb / D1Cc can be made to ask again for the operating language. Refer to *Chapter 6.3 'Permanent Display 1' on page 61*

Should you no longer know where you are in the operating menu, because you cannot read the strange operating language, then press key  10 times. Then you will definitively find yourself in continuous display 1.

## 5.1.2 Selection of the Measured Variable and Measuring Range

### WARNING!

#### Incorrect metering due to incorrect measuring range

Possible consequence: Fatal or serious injuries.

- **The measuring range of the sensor is essential for the measuring range!**
- If the assignment of the measuring range is modified, the settings must be checked in all menus
- If the assignment of the measuring range is changed, the sensor must be recalibrated

With devices, which have not been preconfigured to the customer's specific requirement, the measured variable required has to be selected in the complete operating menu "General Settings / Change Measured Variable". The DULCOMETER® D1Cb / D1Cc then has to be labelled with the label corresponding to the measured variable selected. The relevant labels are enclosed with the DULCOMETER® D1Cb / D1Cc.

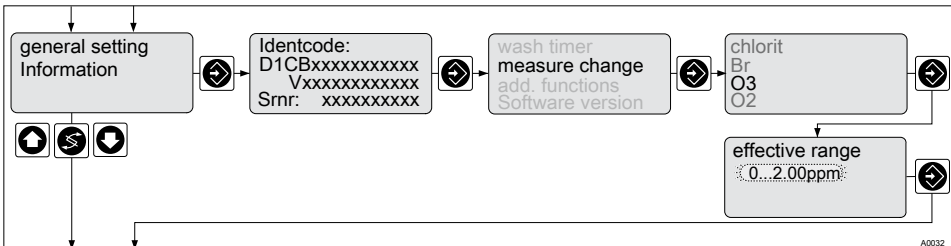


Fig. 24: Selection of measured variable and measuring range

The measuring range required has to be selected and set in the complete operating menu General Settings / Change Measured Variable, see [Chapter 10.6.1 'Setting the Measured Variable/Measuring Range'](#) on page 131.

## 5.2 Activation Code for Extended Functions



### Activation code

Access to further functions can optionally be provided by means of an activation code.

Should you require additional operating literature for these functions, this can be obtained on the homepage of ProMinent Dosiertechnik, Heidelberg.

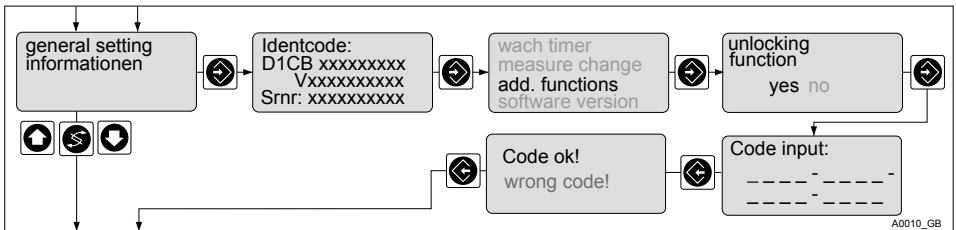


Fig. 25: Activation code / Serial number

The activation code is entered one digit at a time using the and keys. Move to the next position using the key.



The newly activated functions must be configured or parameterised in the relevant menu or new measured variables must be calibrated. Information on this can be found in the relevant complete operating menu.

### 5.2.1 Extended Functions Obtainable with the Activation Code

#### Extended functions

The DULCOMETER® D1Cb / D1Cc controller functionality can be extended or modified by means of a 16-digit activation code. Functions can be enabled several times.



#### D1Cb / D1Cc software upgrade

To provide an activation code, ProMinent requires the 10-digit serial number (Snnr) and the required software upgrade identity code, which can both be found in the table below.

### **! NOTICE!**

#### **Activation code**

When ordering the activation code, it is imperative that you ensure that the serial number (Snr) corresponds exactly to that of the DULCOMETER® D1Cb / D1Cc. Otherwise a chargeable activation code will be provided, which will not work.

### **! NOTICE!**

#### **"Incorrect code" message**

If the code has been entered incorrectly then the "Incorrect code" message will appear. You can enter the activation code as many times as you need to. If this is still not successful, then check the serial number of the controller.



**DULCOMETER® D1Cb / D1Cc software upgrade**

**D1U  
b**      Software default setting

V      Software preset

**Default setting - measured variable**

0      Universal

A      Peracetic acid

B      Bromine

C      Chlorine

D      Chlorine dioxide

F      Fluoride

H      Hydrogen peroxide

I      Chlorite

P      pH

R      ORP

S      0/4-20 mA standard signal general

X      Oxygen

Z      Ozone

L      Conductivity

**Connection of the measured variable**

1\*      Standard signal 0/4-20 mA, all measured variables

5      mV input for pH/redox via guard terminal

**Correction variable**

0      none

2\*      Temperature Pt100/PT1000 (for pH and conductivity)

4\*      Manual temperature input (for pH and conductivity)

\* = chargeable option

## DULCOMETER® D1Cb / D1Cc software upgrade

		<b>Control input</b>	
0		none	
1*		Pause	
		<b>Signal output</b>	
0		none	
1*		Analogue signal output 0/4-20 mA	
		<b>Power activation</b>	
G		Alarm and 2 limit relays	
M*		Alarm and 2 solenoid valve relays	
		<b>Pump activation</b>	
0		none	
2*		2 pumps via pulse frequency	
		<b>Control characteristic</b>	
0		none	
1*		Proportional control	
2*		PID control	
		<b>Language</b>	
00		no default setting	

\* = chargeable option

## 6 Operating diagram/ Display Symbols

### 6.1 Overview of equipment/Control elements

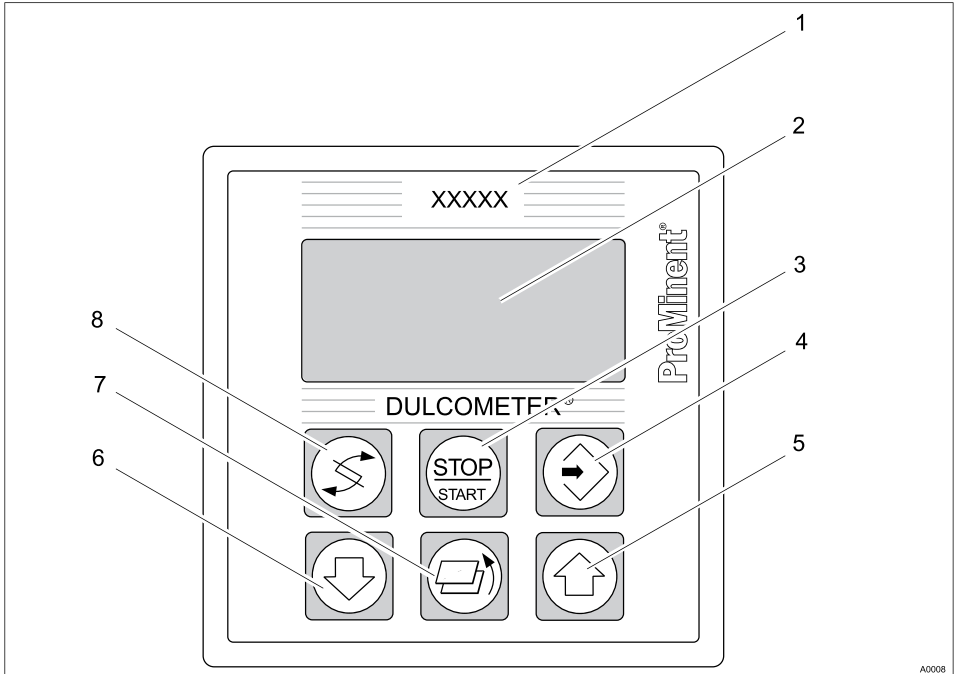


Fig. 26: Overview of equipment/Control elements

Function	Description
1st respective measured variable	Affix the measured variable label here.
2. Display	
3. START/STOP key	Start/Stop the control and metering functions
4. ENTER key	To apply, confirm or save a displayed value or status or to acknowledge an alarm

Function	Description
5. UP key	To increase a displayed numerical value and to change the variables (flashing display). move up in the operating menu.
6. DOWN key	To lower a displayed numerical value and to change the variables (flashing display). To move down in the operating menu.
7. BACK KEY	Back to the continuous display or to the start of the respective setting menu
8. CHANGE key	To change within a menu level and to move from a changeable variable to another changeable variable within a menu option. When inputting numerical values, the cursor moves one space on

## 6.2 Display Symbols

The display of the DULCOMETER® D1Cb / D1Cc uses the following symbols:

Meaning	Comment	Symbol
Limit transgression - relay 1 upper	Symbol left	↑
Limit transgression - relay 1 lower	Symbol left	↓
Limit transgression - relay 2 upper	Symbol right	↑
Limit transgression - relay 2 lower	Symbol right	↓
Metering pump 1 activation off	Symbol left	■
Metering pump 1 activation on	Symbol left	□
Metering pump 2 activation off	Symbol right	■
Metering pump 2 activation on	Symbol right	□
Solenoid valve 1 activation off	Symbol left	▲
Solenoid valve 1 activation on	Symbol left	△

Meaning	Comment	Symbol
Solenoid valve 2 activation off	Symbol right	▴
Solenoid valve 2 activation on	Symbol right	▾
Stop key pressed		○
Manual dosing		M
Fault		ε
Measured value rises very quickly	Trend of measured value display	↑
Measured value rises quickly	Trend of measured value display	↑
Measured value rises slowly	Trend of measured value display	↑
Measured value falls very quickly	Trend of measured value display	↓
Measured value falls quickly	Trend of measured value display	↓
Measured value falls slowly	Trend of measured value display	↓
Measured value steady	Trend of measured value display	↕

### 6.3 Permanent Display 1

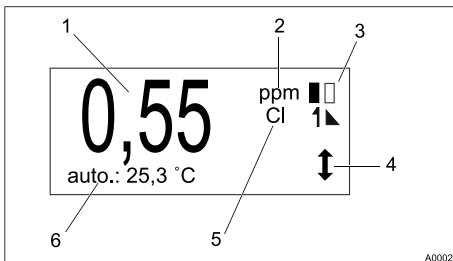


Fig. 27: Permanent Display 1

1. Reading
  2. Mass unit ("ppm" in this example)
  3. Status of the actuators
  4. Display of reading trend - falling / rising
- Not all symbols are visible simultaneously in the permanent display 1. The scope of the symbols depends on what is required.**

5. Measured variable ("chlorine" in this example)

6. Status line

**Not all symbols are visible simultaneously in the permanent display 1. The scope of the symbols depends on what is required.**

### 6.4 Continuous display 2

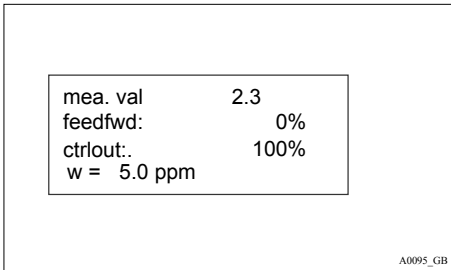





Fig. 28: Continuous display 2

The continuous display 2 shows all the currently required information from the DULCOMETER® D1Cb / D1Cc controller. Switch to other displays by pressing  or  or .

### 6.5 Continuous display 3

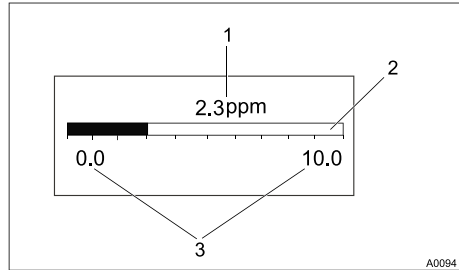










Fig. 29: Continuous display 3

1. Current measured value in plain text
2. Bar graph display shows the current measured value in relation to the lower and upper measured value limits
3. Displays the upper and lower limit of the display

Switch to other displays by pressing  or  or .

To set the lower and upper value (3) press . The left-hand value will flash and can be set using the  or . Confirm the entry with . Likewise, switching between the left- and right-hand values (3) occurs by pressing the key .

This setting only changes the display range of the bar graph, as it were "zooming in" to a smaller range to obtain a better resolution of the display in the main display range of the measurement.



*This setting only changes the display range of the bar graph! A change to the measuring range of the DULCOMETER® D1Cb / D1Cc is not possible using this function.*

### 6.6 Operating diagram




#### ***Access code***

- *Access to the setting menu can be blocked with an access code*
- *If the access code has been correctly selected for a setting menu, then all of the other setting menus are also accessible*

*Fundamentally the continuous displays 1 - 3 and the calibration menu are freely accessible. All of the other menus can be disabled by the access code in such a way that the set values are displayed but cannot be changed. The default value of the access code is "5000".*
- *If no key is pressed within 60 seconds, the device will return to the continuous display 1, the access code is re-enabled and access is restricted*



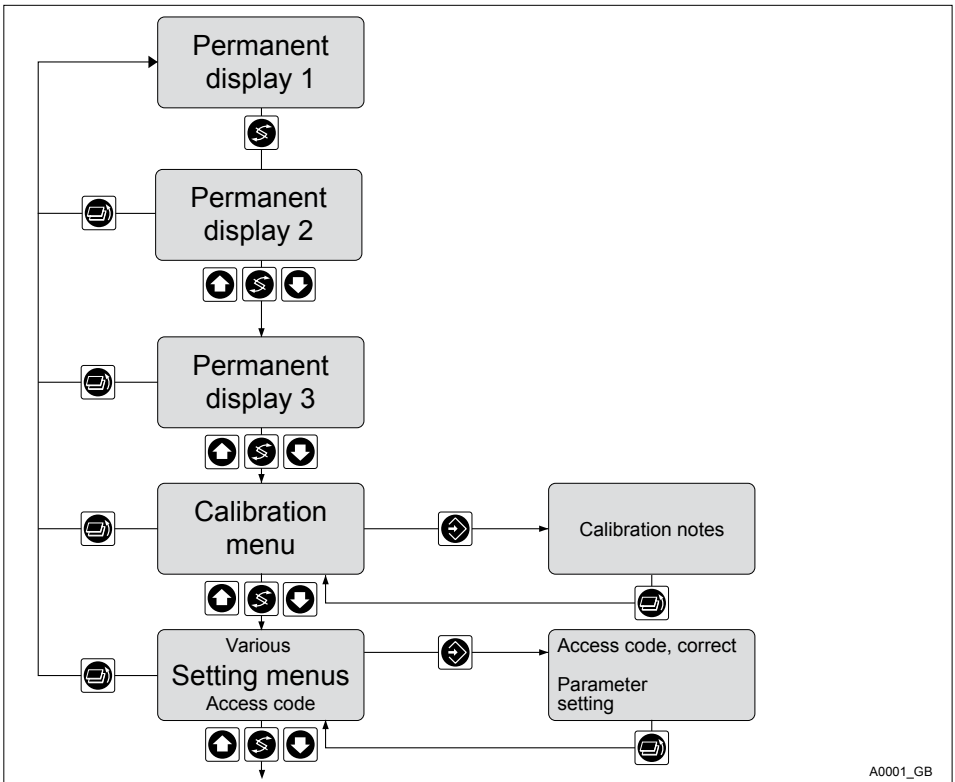

A0001\_GB

Fig. 30: Access code

The number and scope of the setting menu depends on the design of the device.

You can set and change numerical values as follows:

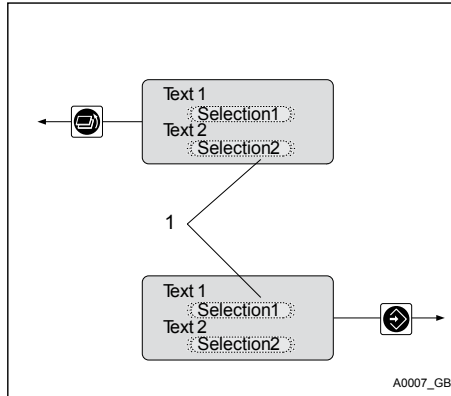










Fig. 31: Settable values flash on and off


1. Settable values flash on and off

You can lower or increase values using the keys  and .

You can switch between the settable values using the  key.




1.  The setpoint (e.g. 7.20 pH) flashes
2.  The the  or  key once  
⇒ The first figure of the numerical value now flashes.
3.  Using the  key you can go back to the figure you want to change



*By pressing the  key multiple times, you can return to the first figure of the numerical value which is to be set.*



*The figure of the numerical value which can be changed flashes.*

4.  You can lower or increase the numerical value using the keys  and 

⇒ You can now save the entire modified numerical value using the  key.

5. ➔ By multiple pressing of the  key you access the next menu point

## 6.7 Reduced / Complete Operating Menu

The DULCOMETER® D1Cb / D1Cc allows settings to be made in two different comprehensive menus (reduced / complete). All of the parameters of the controller are preset and can be changed in the complete operating menu.

The controller is delivered with a restricted operating menu. If adjustments are necessary, the parameters can be changed by switching to the complete operating menu.

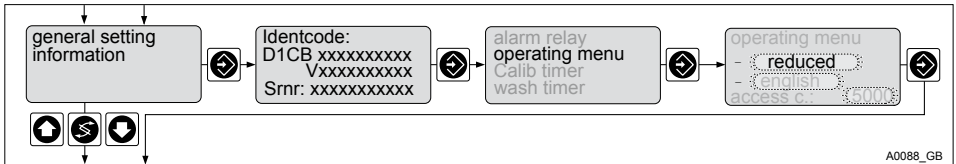


Fig. 32: Reduced / complete changeover

## 6.8 Fault Messages

Any fault messages and notes which arise are shown in the bottom line of the permanent display 1. Faults which have to be acknowledged (acknowledging them switches the alarm relay off) are shown by the  $\Sigma$  symbol.

Faults/notes, which remain after acknowledgement, will be displayed alternately. If a correction variable is being processed, the value will be displayed in the same line as the faults/notes. Faults, which are rectified automatically by changing operating situations, are removed from the permanent display 1 without the need for acknowledgement.

### 6.8.1 Fault display

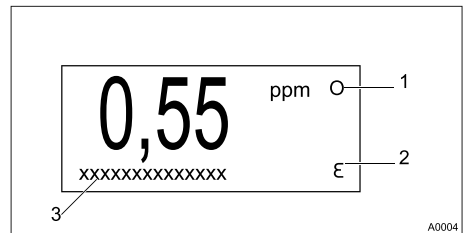


Fig. 33: Fault display

1. Stop function
2. Fault
3. Fault in plain text

## 6.9 General settings

### 6.9.1 Access code

Access to the setting menu can be prevented by an access code. The DULCOMETER® D1Cb / D1Cc is delivered with the access code "5000". Even a security lock is applied using the access code, the calibration menu remains freely accessible.

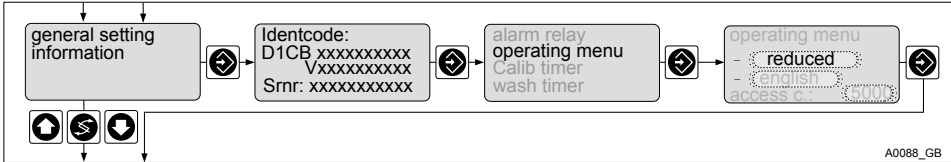


Fig. 34: Access code

	Factory setting	Possible values			Remarks
		Increment	Lower value	Upper value	
Access code	5000	1	0000	9999	

## 7 Measured Variables and Operating Menus for Amperometric Sensors

- **Users' qualification:** instructed persons, see ↪ *Chapter 1.2 'Users' qualifications' on page 10*

## 7.1 Reduced / Complete Operating Menu

The DULCOMETER® D1Cb / D1Cc allows settings to be made in two different comprehensive menus (reduced / complete). All of the parameters of the controller are preset and can be changed in the complete operating menu.

The controller is delivered with a restricted operating menu. If adjustments are necessary, the parameters can be changed by switching to the complete operating menu.

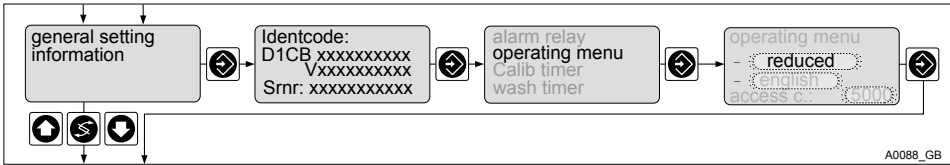



Fig. 35: Reduced / complete changeover

## 7.2 Description of All Amperometric Measured Variables

### WARNING!

#### Danger of incorrect metering

This can result in hazardous incorrect metering

During initial commissioning, the measured variable and the measuring range of the sensor must be set prior to calibration. Refer to  Chapter 5.1.2 'Selection of the Measured Variable and Measuring Range' on page 54


Measured variable	Default measuring range
Chlorine, chlorine dioxide, ozone	2 ppm
Bromine	10 ppm
Oxygen	20 ppm
Peracetic acid	2000 ppm
Hydrogen peroxide	200 ppm
Chlorite	0.5 ppm

The measuring ranges can be selected in the following ppm increments: 0.5, 2, 5, 10, 20, 50, 100, 200, 1000, 2000, 5000, 10000, 20000.

### 7.3 Reduced Operating Menu

The reduced operating menu allows the key parameters to be set. The following overview shows the settings that can be selected:

# Measured Variables and Operating Menus for Amperometric Sensors

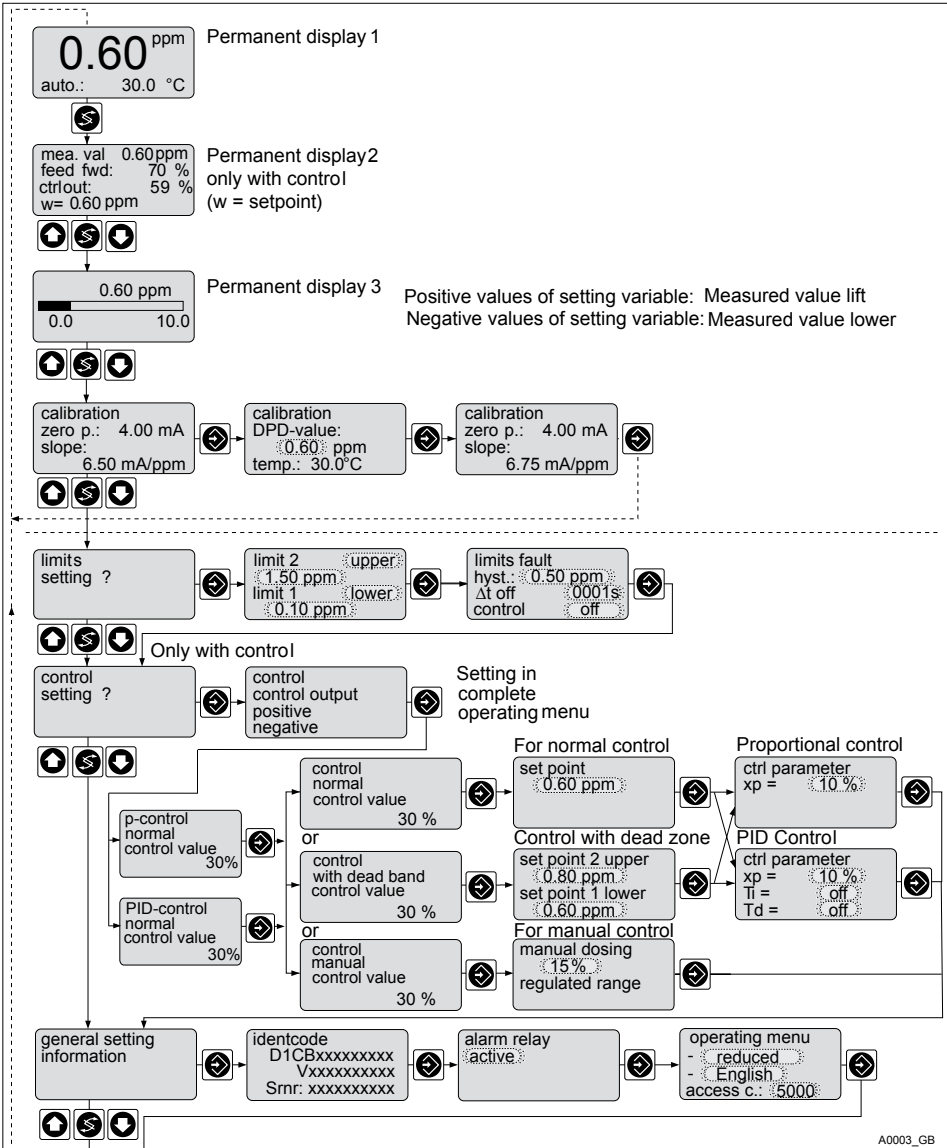

A0003\_GB

Fig. 36: Reduced operating menu



## 7.4 Complete Operating Menu / Description of All Measured Variables

The complete operating menu allows all controller parameters to be set. The following overview shows the settings that can be selected:

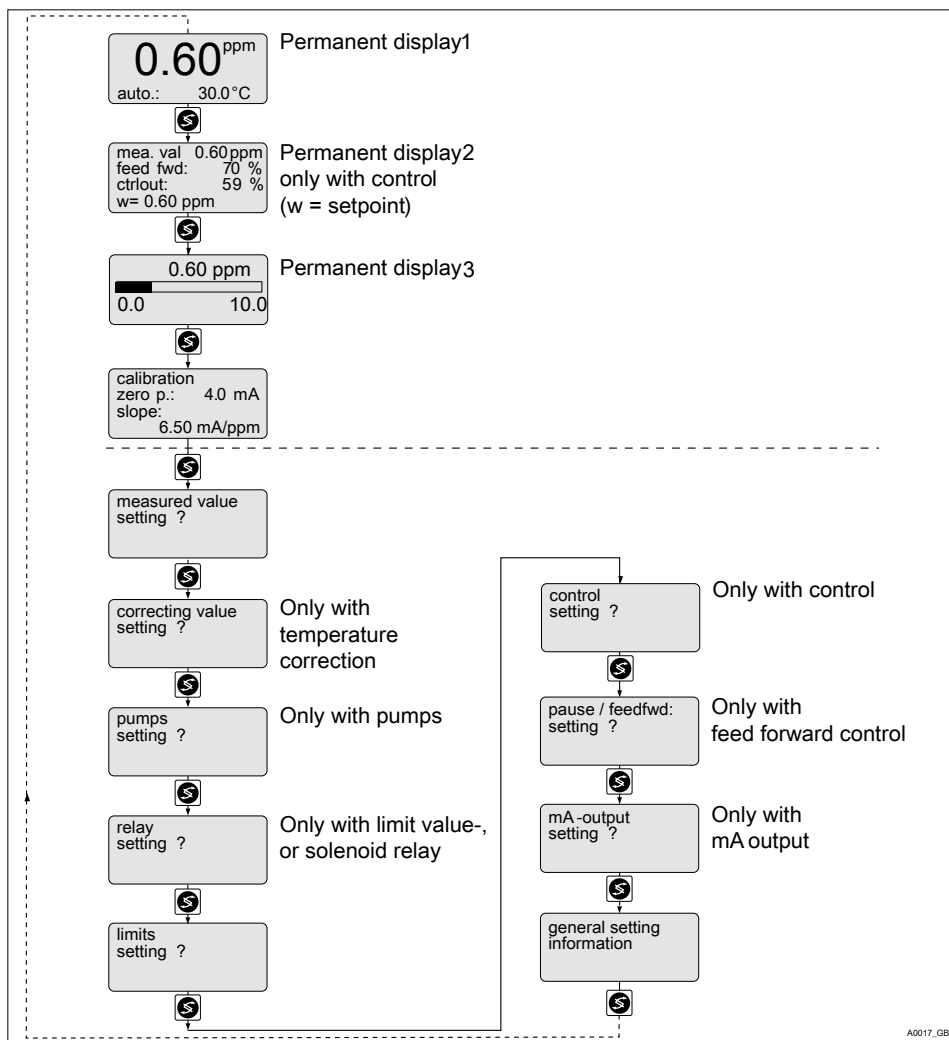


Fig. 37: Complete operating menu

## 7.5 Calibration of All Amperometric Measured Variables

**⚠ WARNING!**

**Danger of incorrect metering**

This can result in hazardous incorrect metering

During initial commissioning, the measured variable and the measuring range of the sensor must be set prior to calibration. Refer to *Chapter 5.1.2 'Selection of the Measured Variable and Measuring Range'* on page 54

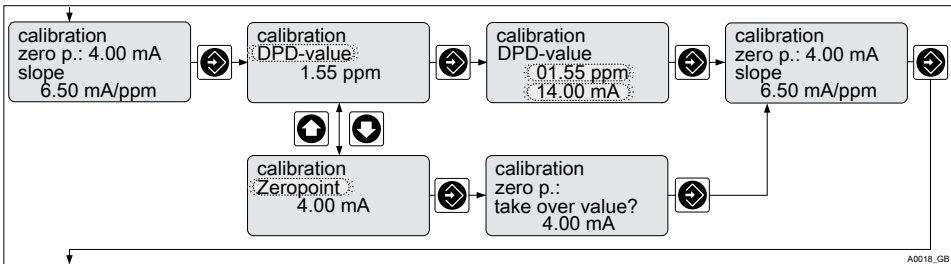


Fig. 38: Calibration of All Amperometric Measured Variables

Error message	Condition	Remarks *
Calibration not possible! Gradient too low	Gradient too low ( $< 20\%$ of standard gradient)	Repeat calibration
Calibration not possible! Gradient too high	Gradient too high ( $> 300\%$ of standard gradient)	Repeat calibration
DPD value too low DPD $> x.xx$ ppm	DPD $< 2\%$ of measuring range	Repeat calibration after addition of metering medium or fit sensor suitable for the process

\* Please also note the operation manual for the respective sensor

---

## Measured Variables and Operating Menus for Amperometric Sensors

---

Error message	Condition	Remarks *
Calibration not possible! Zero point low	< 3 mA (only with 4 - 20 mA sensors)	Check sensor/cable Repeat calibration in water without metering medium
Calibration not possible! Zero point high	> 5 mA > 6 mA for 0.5 ppm chlorite	Check sensor/cable Repeat calibration in water without metering medium

\* Please also note the operation manual for the respective sensor

### 7.6 Calibration of the Sensor for Amperometric Measured Variables

Only the slope can be calibrated in the restricted operating menu of the DULCOMETER® D1Cb / D1Cc.

Both the zero point and the slope can be calibrated in the complete operating menu of the DULCOMETER® D1Cb / D1Cc.

### 7.6.1 Preparation for Calibration of the Sensors for Amperometric Measured Variables



#### CAUTION!

#### Correct sensor operation / Run-in time

Damage to the product or its surroundings

- Correct measuring and dosing is only possible if the sensor is working perfectly
- Please read the operating manual for the sensor
- Please also read the operating manuals for the fittings and other components used
- It is imperative that the run in periods of the sensors are adhered to
- The run in periods should be allowed for when planning commissioning
- It may take a whole working day to run-in the sensor



### ***Necessity of calibrating the zero point***

*Calibration of the zero point is not generally necessary. Calibration of the zero point is only necessary if the sensor is operated at the lower limit of the measuring range or if the 0.5 ppm sensor version is used.*

During the calibration, the DULCOMETER® D1Cb / D1Cc sets the control outputs to "0". Exception: a basic load or a manual control value has been set, this remains active. The mA standard signal outputs are frozen. The measured value frozen at the start of calibration is suggested as a DPD value. The DPD value can be set using the arrow keys. Calibration is only possible if the DPD value is  $\geq 2\%$  of the measuring range of the sensor.

### 7.6.2 Calibration of Zero Point and Slope



#### **NOTICE!**

#### **Prerequisites for correct calibration of the sensor slope**








- The DPD method required by the feed chemical employed will be used
- The run in period for the sensor has been adhered to
- There is permitted and constant flow at the in-line probe housing
- There is temperature balance between the sensor and the sample water
- There is a constant pH value in the permitted range

### Calibration of amperometric sensors: slope (in the reduced and complete operating menu)

The sensor is fitted, flushed with sample water and connected electrically to the DULCOMETER® D1Cb / D1Cc and run-in.

There has to be adequate feed chemical in the sample water for calibration (> 2% of the measuring range of the sensor).

Remove sample water directly at the measuring point and determine the content of metering medium in the sample water in "ppm" using an appropriate reference method (e.g. DPD, titration etc.). Enter this value as follows at the DULCOMETER® D1Cb / D1Cc:

1. ➤ Select Calibration menu. Then press 
  - ⇒ The current measured value will now be frozen.
2. ➤ Take a sample of water and perform a reference measurement within 15 minutes
3. ➤ Select "DPD value" of unit to be calibrated using the  key
4. ➤ Continue with 
5. ➤ If necessary, match the flashing ppm value to the value determined with the measurement using the keys, ,  and 
  - ⇒ The mA value of the sensor shown in this display now corresponds to the measured value in "ppm".
6. ➤ Then press the following key twice 

- ⇒ The display now shows the value determined for the zero point and slope. Refer to the Error Message table should an error be displayed. ↪ *Table on page 74*











### ***Necessity of calibrating the zero point***

*Calibration of the zero point is not generally necessary. Calibration of the zero point is only necessary if the sensor is operated at the lower limit of the measuring range or if the 0.5 ppm sensor version is used.*

### Calibration of amperometric sensors: Zero point (only in the complete operating menu)

A container with water, which is free of additives that could falsify the measured result, is needed for calibration. Immerse the dismantled, but still electrically connected to the DULCOMETER® D1Cb / D1Cc, sensor in this water. Use the sensor to stir the water for approx. 5 minutes until the measured value displayed at the DULCOMETER® D1Cb / D1Cc is steady and close to "0".

1. ➤ Select Calibration menu. Then press 
2. ➤ Select "Zero point" of unit to be calibrated using the  key
3. ➤ Continue with 
  - ⇒ A prompt is shown in the display
4. ➤ Confirm prompt with the key 
5. ➤ Continue with 
6. ➤ Apply the "zero point" displayed during calibration using the  key
7. ➤ Then press 
  - ⇒ Display shows the values determined.
8. ➤ Then press 
  - ⇒ Refer to the Error Message table should an error be displayed. ↪ *Table on page 74*

### NOTICE!

Then definitively calibrate the slope with a suitable reference method (e.g. DPD. titration etc.).

## 7.7 Setting the Measured value



### WARNING!

#### Incorrect metering due to incorrect metering range

Possible consequence: Fatal or serious injuries.

- **The measuring range of the sensor is essential for the measuring range!**
- If the assignment of the measuring range is modified, the settings must be checked in all menus
- If the assignment of the measuring range is changed, the sensor must be recalibrated
- The relevant information can be found in the operating manual for the sensor/ measuring equipment

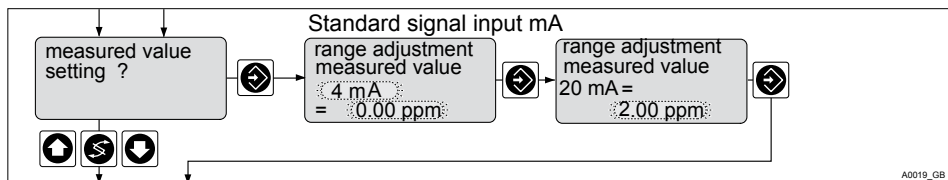


Fig. 39: Measured value

This setting is solely for matching the DULCOMETER® D1Cb / D1Cc to the sensors of third party suppliers. Sensors provided by third party providers may have measuring ranges, which deviate from the default settings of the DULCOMETER® D1Cb / D1Cc.

To match a sensor from Prominent to the DULCOMETER® D1Cb / D1Cc, please only use the menu under 'General Settings', see [Chapter 5.1.2 'Selection of the Measured Variable and Measuring Range'](#) on page 54

## 7.8 Correcting value



Only necessary when using the DULCOTEST® CDP sensor for chlorine dioxide ClO<sub>2</sub>.

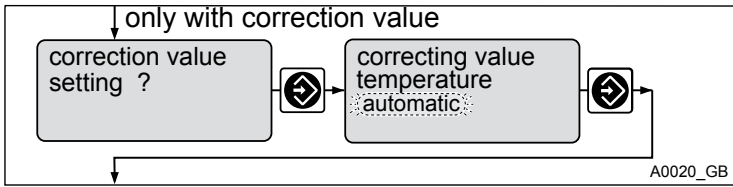






Fig. 40: Correcting value

The correction variable compensates for the effect of the temperature of the medium on the measured value. The correction variable is the temperature of the medium to be measured. The temperature of the medium affects the value to be measured. For amperometric sensors only necessary when using the DULCOTEST® CDP sensor for chlorine dioxide ClO<sub>2</sub>.

### Operating modes

- Off: No temperature compensation takes place.
  - For measurements which do not require temperature compensation.
- Automatic: The DULCOMETER® D1Cb / D1Cc evaluates the temperature signal of the connected temperature sensor.
  - For measurements with temperature sensors, which deliver a temperature signal which can be evaluated by the DULCOMETER® D1Cb / D1Cc (Pt100/Pt1000) (0 -100 °C).
- Manual: The temperature of the medium to be measured has to be measured by the user. The measured value is then entered using the keys: ,  and  into the DULCOMETER® D1Cb / D1Cc and saved by pressing the key .

  - For measurements where the medium to be measured has a constant temperature, which has to be taken into account in the control process.



## 8 Measured Variables and Operating Menus for Potentiometric Sensors

- **Users' qualification:** instructed persons, see ↗ *Chapter 1.2 'Users' qualifications' on page 10*

### Measured variables pH, ORP, fluoride



#### CAUTION!

#### Influence of temperature on the pH or fluoride measurement

Possible consequence: Slight or minor injuries. Material damage.

Temperature changes in the sample water lead to a change in the slope of the calibration lines (pH, fluoride) and to a displacement of the zero point with pH sensors or the standard potential  $E_S$  for fluoride sensors.

Measure to be taken to avoid this danger:

- The pH or fluoride measurement should only be carried out in the *[Temperature Correction Value automatic]* setting
- The DULCOMETER® D1Cb / D1Cc then automatically compensates for both effects when connecting a temperature sensor (Pt 100/Pt 1000)

### 8.1 Reduced / Complete Operating Menu

The DULCOMETER® D1Cb / D1Cc allows settings to be made in two different comprehensive menus (reduced / complete). All of the parameters of the controller are preset and can be changed in the complete operating menu.

The controller is delivered with a restricted operating menu. If adjustments are necessary, the parameters can be changed by switching to the complete operating menu.

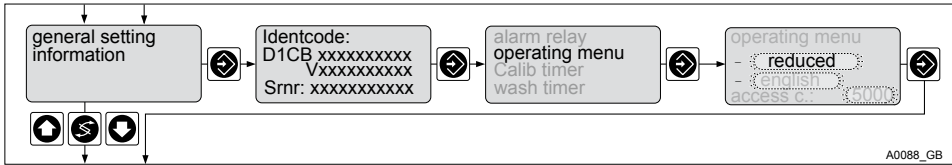



Fig. 41: Reduced / complete changeover

### 8.2 Description of pH, Redox and Fluoride Measured Variables

#### WARNING!

##### Danger of incorrect metering

This can result in hazardous incorrect metering

During initial commissioning, the measured variable and the measuring range of the sensor must be set prior to calibration. Refer to  Chapter 5.1.2 'Selection of the Measured Variable and Measuring Range' on page 54

pH Measured variable	Typical measuring range
Measuring range	- 500 mV ... + 500 mV
Display range	At least pH -1.45 ... 15.45
Reference temperature	+25°C
Resolution	0.01 pH


Redox measured variable	Typical measuring range
Measuring range	-1000 mV ... + 1000 mV
Resolution	1 mV

Fluoride measured variable	Measuring range
Measuring range	0....10 ppm 0.... 99.99 ppm
Resolution	0.01 ppm

### 8.3 Reduced pH / Redox / Fluoride Operating Menu

The reduced operating menu allows the key parameters to be operated. The following overview shows the settings that can be selected (shown here for pH as the measured variable):

# Measured Variables and Operating Menus for Potentiometric Sensors

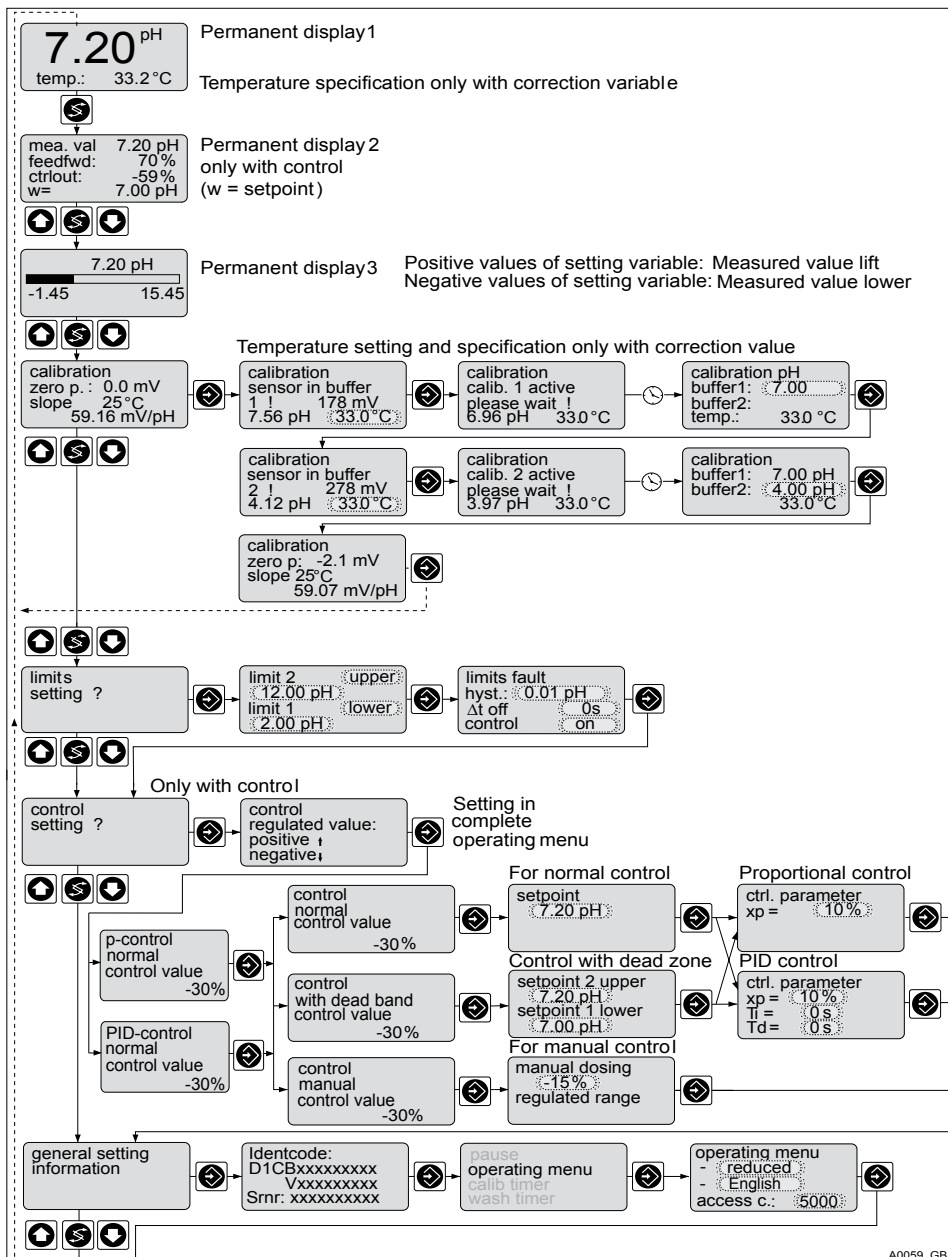


*Fig. 42: Reduced pH / redox / fluoride operating menu (shown with the example of pH)*

### 8.4 Complete Operating Menu/Description of pH / ORP / Fluoride

The complete operating menu is for setting all the parameters of the DULCOMETER® D1Cb / D1Cc. The following overview shows the settings that can be selected: (shown here for pH as the measured variable)

# Measured Variables and Operating Menus for Potentiometric Sensors

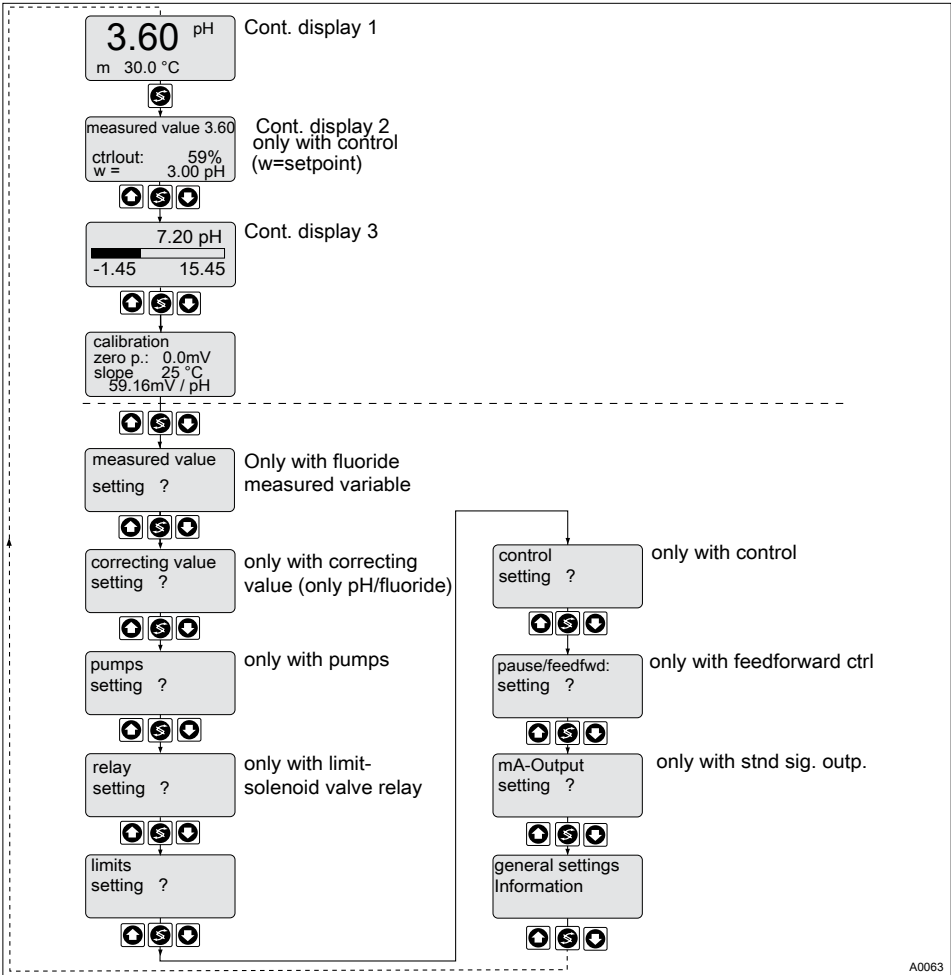

A0063

Fig. 43: Complete pH / ORP / fluoride operating menu

### 8.5 Calibration of pH, ORP and Fluoride Sensors



#### **WARNING!**

##### **Incorrect metering due to incorrect metering range**

Possible consequence: Fatal or serious injuries.

- **The measuring range of the sensor is essential for the measuring range!**
- If the assignment of the measuring range is modified, the settings must be checked in all menus
- If the assignment of the measuring range is changed, the sensor must be recalibrated

During calibration, the DULCOMETER® D1Cb / D1Cc, see *Chapter 1.2 'Users' qualifications' on page 10* sets the control outputs to '0'. Exception: a basic load or a manual control value has been set. This remains active. The mA standard signal outputs are frozen.

When calibration/testing has been completed successfully, all of the error checks relating to the measured value are restarted. The DULCOMETER® D1Cb / D1Cc stores the determined data for zero point and slope. Refer to *Chapter 10.6.2.7 'Calibration Logbook' on page 133*



#### **CAUTION!**

##### **Correct sensor operation / Run-in time**

Damage to the product or its surroundings

- Correct measuring and dosing is only possible if the sensor is working perfectly
- Please read the operating manual for the sensor
- It is imperative that the run in periods of the sensors are adhered to
- The run in periods should be allowed for when planning commissioning

## 8.5.1 Description of the Calibration of pH Sensors

### 8.5.1.1 2-Point Calibration



#### 2-Point Calibration

Recommended as the standard method



#### Calibration of pH sensors with temperature as the correction variable

When calibrating with temperature as the correction variable, the temperature of the buffer solution must be set in "manual" operating mode before calibration.

In "Automatic" operating mode, the temperature sensor must be immersed in the buffer solution. The calibration values are then calculated whilst taking into consideration the buffer temperature.

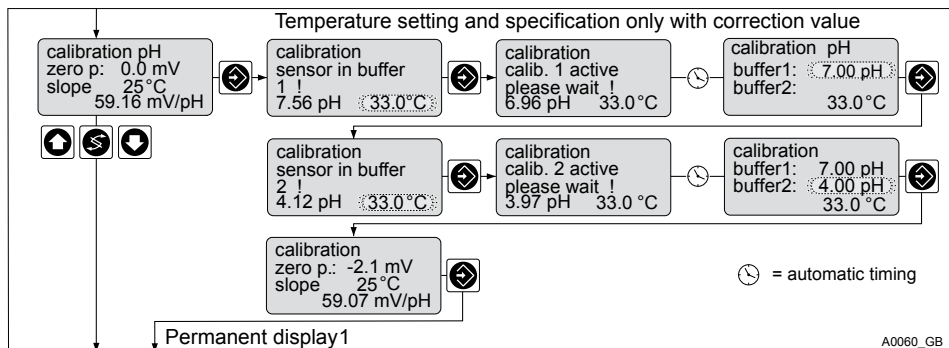


Fig. 44: Calibration of pH sensors
















---

## Measured Variables and Operating Menus for Potentiometric Sensors

---

Two test containers with a buffer solution are required for calibration. The pH value of the buffer solutions should be at least 2 pH values apart. The sensor should be rinsed thoroughly with water when changing the buffer solution.

1. ▶ Select Calibration menu 
2. ▶ Immerse sensor in test container 1 with buffer solution (e.g. pH 7)
3. ▶ Move the sensor gently until the pH value displayed no longer changes
4. ▶ Then press 
  - ⇒ Calibration is running
  - A buffer value is suggested once the waiting time has expired.
5. ▶ If necessary adjust the pH value displayed using keys ,  and  to the actual value of the buffer solution in test container 1
6. ▶ Then press 
7. ▶ Remove the sensor, rinse thoroughly in water and then dry with a cloth (pad dry, don't rub!)
8. ▶ Immerse sensor in test container 2 with buffer solution (e.g. pH 4)
9. ▶ Move the sensor gently until the pH value displayed no longer changes
10. ▶ Then press 
  - ⇒ Calibration is running
  - A buffer value is suggested once the waiting time has expired.
11. ▶ If necessary adjust the pH value displayed using keys ,  and  to the actual value of the buffer solution in test container 2
12. ▶ Then press 
  - ⇒ The settings recorded will be displayed.
13. ▶ If the calibration result is correct, confirm with 
  - ⇒ The new calibration is now applied.

Should the result of the calibration lie outside of the specified error limits, an error message will appear, see  *Chapter 8.5.3 'Calibration of pH Sensors. Description of the Error Messages' on page 91*. In this case the current calibration will not be applied.

### 8.5.1.2 1-Point Calibration



#### 1-Point Calibration

*Recommended only for special applications e.g. swimming pool water*



#### Calibration of pH sensors with temperature as the correction variable

*When calibrating with temperature as the correction variable, the temperature of the buffer solution must be set in "manual" operating mode before calibration.*

*In "Automatic" operating mode, the temperature sensor must be immersed in the buffer solution. The calibration values are then calculated whilst taking into consideration the buffer temperature.*

One test container with a buffer solution is required for calibration.

1. ➤ Select Calibration menu
2. ➤ Immerse the sensor in the test container with buffer solution (e.g. pH 7)
3. ➤ Move the sensor gently until the pH value displayed no longer changes
4. ➤ Then press
  - ⇒ Calibration is running
  - A buffer value is suggested once the waiting time has expired.
5. ➤ If necessary adjust the pH value displayed using keys , and to the actual value of the buffer solution in the test container
6. ➤ Then press
7. ➤ Then press
  - ⇒ The settings recorded will be displayed.
8. ➤ If the calibration result is correct, confirm with
  - ⇒ The new calibration is only now applied.

Should the result of the calibration lie outside of the specified error limits, an error message will appear, see *Chapter 8.5.3 'Calibration of pH Sensors. Description of the Error Messages' on page 91*. In this case the current calibration will not be applied.

### 8.5.2 Calibration of pH Sensors. Description of the Setting Ranges

Setting	Possible values				Remarks
	Starting value	Increment	Lower value	Upper value	
Calibration temperature	Reading	0.1 °C	0 °C	100 °C	
Buffer values	Reading (whole digit rounded up)	0.01 pH	-1.45 pH	15.45 pH	Error message if the two buffers lie too close to each other (<2 pH values)

### 8.5.3 Calibration of pH Sensors. Description of the Error Messages

Error message	Condition	Effect	
Buffer gap too small	$\Delta\text{buffer} < 2 \text{ pH}$	During the calibration process: recalibrate buffer 2! Back to the permanent display	
pH zero point low	$< -60 \text{ mV}$	Basic load metering	Note: old zero point and gradient remain
pH zero point high	$> +60 \text{ mV}$	Basic load metering	Note: old zero point and gradient remain
pH gradient low	$< 40 \text{ mV/pH}$	Basic load metering	Note: old zero point and gradient remain
pH gradient high	$> 65\text{mV/pH}$	Basic load metering	Note: old zero point and gradient remain
pH reading unsteady			Note: old zero point and gradient remain
°C reading unsteady			Note: old zero point and gradient remain

**The following applies to all error messages: eliminate the source of the error and repeat calibration.**

### 8.5.4 Testing the Redox Sensor

#### CAUTION!

##### Correct sensor operation / Run-in time

Damage to the product or its surroundings

- Correct measuring and metering is only possible if the sensor is working perfectly
- Please read the operating manual for the sensor
- It is imperative that the run-in times of the sensors are adhered to
- The run-in times should be allowed for when planning initial operation

#### NOTICE!

##### Testing the Redox Sensor

With redox measured variables, the sensor is not calibrated but tested according to its design

- Observe any notification of abnormal behaviour when testing the redox sensor
- Should the test not be successful, replace the redox sensor

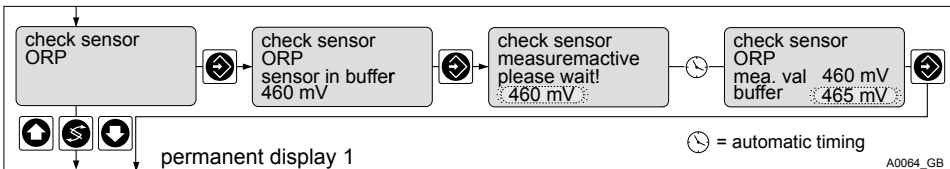









Fig. 45: Testing redox sensors

#### 8.5.4.1 Description of the Testing of Redox Sensors

A container with a redox buffer solution (e.g. 465 mV) is needed for testing.

1.  Select the Test menu 

2. ▶ Immerse redox sensor in the test container with redox buffer solution (e.g. 465 mV)
3. ▶ Start test with 
  - ⇒ Test is running.  
  
A buffer value is suggested once the waiting time has expired.
4. ▶ Adjust displayed value of "buffer" (flashing) using ,  and  to the mV value of the redox buffer solution in the test container and confirm the value with 
  - ⇒ The D1Cb displays the status message of the redox sensor in plain text. If the redox sensor is functioning correctly, permanent display 1 will be displayed directly
5. ▶ If the redox sensor is unclean or defective, the redox sensor should be cleaned, as described in the redox sensor operating manual, or alternatively replaced

Should the result of the calibration lie outside of the specified error limits, an error message will appear, see

☞ *Chapter 8.5.4.3 'Testing Redox Sensors. Description of the Error Messages' on page 94*

### 8.5.4.2 Testing Redox Sensors Buffer Values Tables

Table: Possible buffer values

Setting	Starting value	Possible values			Remarks
		Increment	Lower value	Upper value	
Buffer values	Reading	1 mV	-1,500 mV	+1,500 mV	
185-265 mV	220 mV				
425-505 mV	465 mV				

### 8.5.4.3 Testing Redox Sensors. Description of the Error Messages

Table: Possible error messages when testing redox sensors

Error message	Condition	Effect
Reading high	Reading 40 mV > buffer	Back to the permanent display Basic load metering
Reading low	Reading 40 mV < buffer	Back to the permanent display Basic load metering

## 8.5.5 Description of the Calibration of Fluoride Sensors

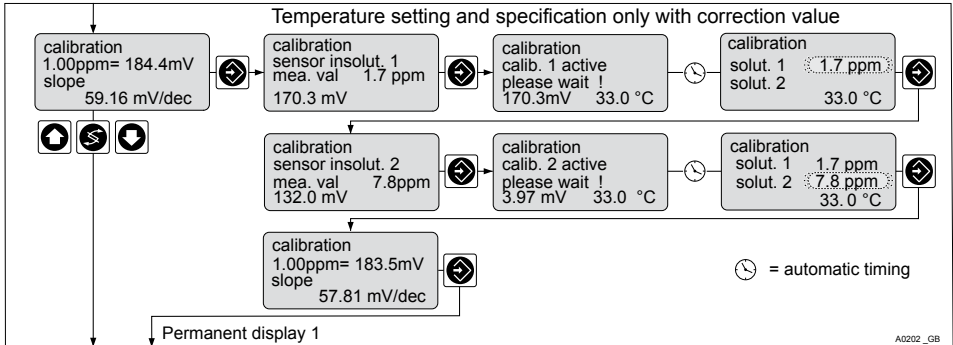



Fig. 46: Calibrating the fluoride sensor

### 8.5.5.1 Description of the Calibration of Fluoride Sensors

#### Temperature correction variable

When calibrating with temperature as the correction variable, the temperature of the buffer solution has to be set. in "manual" operating mode before calibration. Refer to  Chapter 8.6 'Temperature correction value for pH and fluoride sensors' on page 99

In "Automatic" operating mode, the temperature sensor must be immersed in the buffer solution. The calibration values are then calculated allowing for the temperature.

### 8.5.5.1.1 Description of 2-Point Calibration for Fluoride Sensors

Material required for calibration of fluoride sensors

- Two test containers with calibrating solution
- A thermometer for measuring in fluids (in "Temperature Correction Value manual" operating mode)

Two test containers with calibrating solution are required for calibration. The fluoride content of the calibrating solutions should be at least 0.5 ppm F apart from each other. The sensor should be rinsed thoroughly with fluoride-free water when changing the calibrating solution.

#### 1. Select Calibration menu










- ⇒ In "Temperature Correction Value manual" operating mode, the calibration display appears and the temperature value flashes.

---










## Measured Variables and Operating Menus for Potentiometric Sensors

---


In "Temperature Correction Value automatic" operating mode the calibration display appears

2. ➤ Measure the temperature of the calibrating solution 1 using the thermometer (only in "Temperature Correction Value manual" operating mode)
3. ➤ Enter the determined value for the calibration solution temperature using the keys ,  and  into the DULCOMETER® D1Cb / D1Cc
4. ➤ Confirm entry with the key 
  - ⇒ The DULCOMETER® D1Cb / D1Cc allows for the actual temperature of the calibration solution during the calibration.
5. ➤ Immerse the fluoride sensor in calibration solution 1 and wait until the mV value displayed remains steady (fluctuation of < 0.05 mV/min)
6. ➤ Start the calibration process by pressing 
  - ⇒ Calibration is running
7. ➤ Using the keys ,  and  enter the determined concentration for the calibration solution in ppm into the DULCOMETER® D1Cb / D1Cc
8. ➤ Confirm the ppm value by pressing 
  - ⇒ In "Temperature Correction Value manual" operating mode, the calibration display appears and the temperature value flashes.

In "Temperature Correction Value automatic" operating mode the calibration display appears

9. ➤ Measure the temperature of the calibrating solution 2 using the thermometer (only in "Temperature Correction Value manual" operating mode)
10. ➤ Prepare for calibration in calibrating solution 2
11. ➤ Enter the determined value for the calibration solution temperature using the keys ,  and  into the DULCOMETER® D1Cb / D1Cc
12. ➤ Confirm entry with the key 
  - ⇒ The DULCOMETER® D1Cb / D1Cc allows for the actual temperature of the calibration solution during the calibration.
13. ➤ The fluoride sensor should be rinsed thoroughly with fluoride-free water when changing the calibrating solution
14. ➤ Immerse the fluoride sensor in calibration solution 2 and wait until the mV value displayed remains steady (fluctuation of < 0.05 mV/min)
15. ➤ Start the calibration process by pressing 
  - ⇒ Calibration is running.
16. ➤ Using the keys ,  and  enter the determined concentration for the calibration solution in ppm into the DULCOMETER® D1Cb / D1Cc
17. ➤ Confirm the ppm value by pressing 















- ⇒ The display of the DULCOMETER® D1Cb / D1Cc shows the result of the calibration. If the calibration result is correct, confirm by pressing .

### 8.5.5.1.2 1-Point Calibration of the Fluoride Sensor

#### Calibration of fluoride. Description of 1-point calibration





One container with a calibrating solution is required for calibration.

1.  Select Calibration menu 
  - ⇒ In "Temperature Correction Value manual" operating mode, the calibration display appears and the temperature value flashes.  
  
In "Temperature Correction Value automatic" operating mode the calibration display appears
2.  Measure the temperature of the calibrating solution 1 using the thermometer (only in "Temperature Correction Value manual" operating mode)
3.  Enter the determined value for the calibration solution temperature using the keys ,  and  into the DULCOMETER® D1Cb / D1Cc
4.  Confirm entry with the key 
  - ⇒ The DULCOMETER® D1Cb / D1Cc allows for the actual temperature of the calibration solution during the calibration.
5.  Immerse the fluoride sensor in calibrating solution 1 and wait until the mV value displayed remains steady (fluctuation of < 0.05 mV/min)
6.  Start the calibration process by pressing 
  - ⇒ Calibration is running

---

## Measured Variables and Operating Menus for Potentiometric Sensors

---

7. → Using the keys ,  and  enter the determined concentration for the calibration solution in ppm into the DULCOMETER® D1Cb / D1Cc
8. → Confirm the ppm value by pressing 

## 8.6 Temperature correction value for pH and fluoride sensors



### CAUTION!

#### Influence of temperature on the pH or fluoride measurement

Possible consequence: Slight or minor injuries. Material damage.

Temperature changes in the sample water lead to a change in the slope of the calibration lines (pH, fluoride) and to a displacement of the zero point with pH sensors or the standard potential  $E_S$  for fluoride sensors.

Measure to be taken to avoid this danger:

- The pH or fluoride measurement should only be carried out in the *[Temperature Correction Value automatic]* setting
- The DULCOMETER® D1Cb / D1Cc then automatically compensates for both effects when connecting a temperature sensor (Pt 100/Pt 1000)

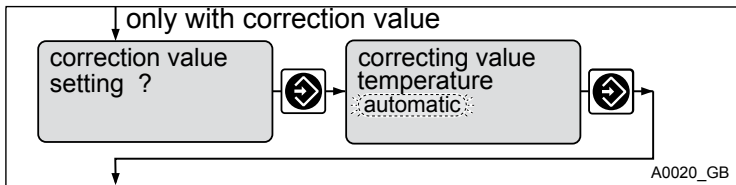


Fig. 47: Temperature correction value for pH and fluoride sensors

Temperature correction value for pH and fluoride sensors in line with the identity code:

	Possible values		
As per identity code	Increment	Lower value	Upper value
0	off		
2	off Manual Automatic		
4	off Manual		

---


## Measured Variables and Operating Menus for Potentiometric Sensors

---


### Temperature correction value for pH and fluoride sensors

		Possible values		
	Factory setting	Increment	Lower value	Upper value
Manual temperature compensation	25 °C	0.1 °C	0 °C	100 °C

### 9 Measured Variables and Operating Menus for the Standard Signal General

- **Users' qualification:** instructed persons, see  *Chapter 1.2 'Users' qualifications' on page 10*

#### 9.1 Explanation of the Standard Signal General

The measured variable "Standard Signal General" of the DULCOMETER® D1Cb / D1Cc is used to connect sensors from third party providers, which send a linear mA signal, to the DULCOMETER® D1Cb / D1Cc. The DULCOMETER® D1Cb / D1Cc is thus preconditioned to be able to measure and control a number of physical measured variables, using appropriate sensors, see  *Table on page 105.*



#### Adjusting the sensor output signal

To match the DULCOMETER® D1Cb / D1Cc to the output signal from the sensor or measuring device you must carry out the following steps:

#### NOTICE!

##### **Linear characteristic line**



As the DULCOMETER® D1Cb / D1Cc can only process linear characteristic lines, only sensors/measuring devices can be connected, which emit a linear signal.

1.  Changing the DULCOMETER® D1Cb / D1Cc over to the complete operating menu
2.  Set the required physical unit (measured variable)



#### **Display tolerances**

*With sensors or with output signals of measuring devices, which do not have to be calibrated or with which calibration has to be done in the sensor/measuring device, the display tolerances must then be calibrated between the sensor or measuring device and the DULCOMETER® D1Cb / D1Cc.*

3.  To do so, select the menu "Set measured value", see  *Chapter 9.4 'Setting the Reading' on page 104.*

4. ➔ The measuring range limit of 0/4 mA and 20 mA can be adjusted by raising and/or lowering the measured values
- ⇒ The limits of the measuring range are adjusted in order to calibrate the display tolerance between the sensor or measuring device and the DULCOMETER® D1Cb.

**! NOTICE!**

**Calibration**

ProMinent also offers the possibility of one-point or two-point calibration of the "standard signal general" measured variable. This calibration option should only be used if the manufacturer of the sensor or measuring equipment describes or permits this in the operating manual for the sensor or measuring equipment.

## 9.2 Changing the Measured Variable



### WARNING!

#### Incorrect metering due to incorrect measured variable

Possible consequence: Fatal or serious injuries

- **The measured variable/measuring range of the sensor is essential for the measured variable/measuring range!**
- If the measured variable/measuring range is changed, the sensor must be recalibrated
- If the measured variable/measuring range is changed, the set points and limit values will be changed to the associated starting values!
- If the measured variable/measuring range is changed, the settings in all of the menus must be checked

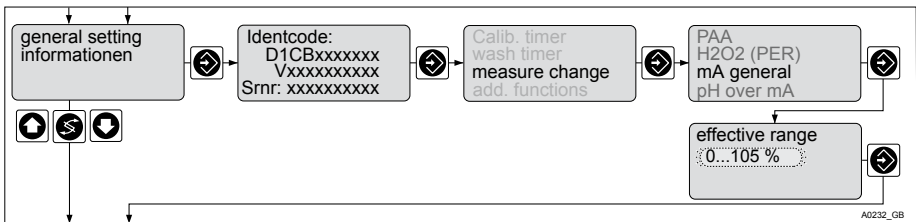


Fig. 48: Changing "Standard signal general" measured variable

For possible measured variables see Table on page 105.

### 9.3 Reduced / Complete Operating Menu

The DULCOMETER® D1Cb / D1Cc allows settings to be made in two different comprehensive menus (reduced / complete). All of the parameters of the controller are preset and can be changed in the complete operating menu.

The controller is delivered with a restricted operating menu. If adjustments are necessary, the parameters can be changed by switching to the complete operating menu.

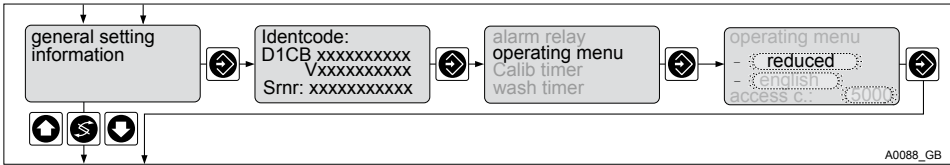


Fig. 49: Reduced / complete changeover

### 9.4 Setting the Reading

**WARNING!**

**Incorrect metering due to incorrect measured variable**

Possible consequence: Fatal or serious injuries

- **The measured variable/measuring range of the sensor/measuring device is essential for the measured variable/measuring range!**
- If the measured variable/measuring range is changed, the sensor must be recalibrated
- If the measured variable/measuring range is changed, the set points and limit values will be changed to the associated starting values!
- If the measured variable/measuring range is changed, the settings in all of the menus must be checked

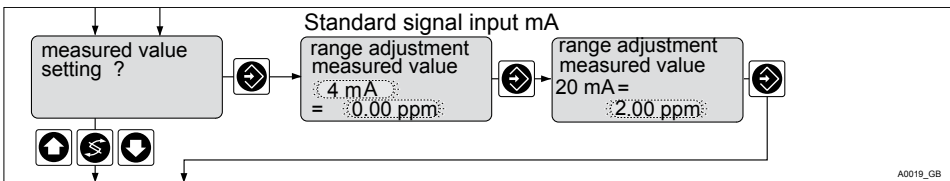


Fig. 50: Reading



**Range assignment table**

	Starting value	Possible values		
		Increment	Lower value	Upper value
Lower signal limit	4 mA	0 mA		
		4 mA		
Assigned measuring range*	0 - 100.0 %	0.1 %	-5 %	105 %
	0 - 20.00 mA	0.01 mA	-1.00 mA	21.00 mA

\*= for other measuring ranges see [↪ Table on page 105](#)

**9.5 Description of All Standard Signal Measured Values/Measured Variables**

Measured variable	Possible values			Measuring range*
	Increment	Lower value	Upper value	
Measuring signal	0.1%	-5,0 %	105,0 %	100 %
	0.01 mA	-1.00 mA	21.00 mA	20 mA
Filling level	0.01 m	0.00 m	31.50 m	30 m
	0.1 %	0.0 %	105,0 %	100 %
Pressure	0.001 bar	0.000 bar	1.050 bar	1.000 bar
	0.001 bar	0.000 bar	5.250 bar	5.000 bar
	0.01 bar	0.00 bar	10.50 bar	10.00 bar
	0.1 bar	0.0 bar	105.0 bar	100.0 bar
	0.1 psi	0.0 psi	105.0 psi	100 psi
	1 psi	0 psi	1050 psi	1000 psi

\* Maximum set point that can be set

## Measured Variables and Operating Menus for the Standard Signal General

Measured variable	Possible values			Measuring range*
	Increment	Lower value	Upper value	
Flow rate	0.001 m <sup>3</sup> /h	0.000 m <sup>3</sup> /h	10.00 m <sup>3</sup> /h	9.999 m <sup>3</sup> /h
	0.1 m <sup>3</sup> /h	0.0 m <sup>3</sup> /h	105.0 m <sup>3</sup> /h	100 m <sup>3</sup> /h
	1 m <sup>3</sup> /h	0 m <sup>3</sup> /h	1,050 m <sup>3</sup> /h	1,000 m <sup>3</sup> /h
	0.1 gal/h	0.0 gal/h	105.0 gal/h	100 gal/h
	1 gal/h	0 gal/h	1050 gal/h	1000 gal/h
Concentration	1 ppm	0 ppm	1050 ppm	1000 ppm
Relative humidity	0.1 % rel. humidity	0.0 % rel. humidity	105.0 % rel. humidity	100 % rel. humidity
mA signal	0.01 mA	0.00 mA	21.00 mA	20 mA
	0.01 mA	4.00 mA	21.00 mA	20 mA
Turbidity value	1 NTU	0 NTU	10 NTU	10 NTU
	1 NTU	0 NTU	105 NTU	100 NTU
	1 NTU	0 NTU	2100 NTU	2000 NTU
* Maximum set point that can be set				

### 9.6 Reduced Operating Menu

The reduced operating menu allows the key parameters to be set. The following overview shows the settings that can be selected:

# Measured Variables and Operating Menus for the Standard Signal General

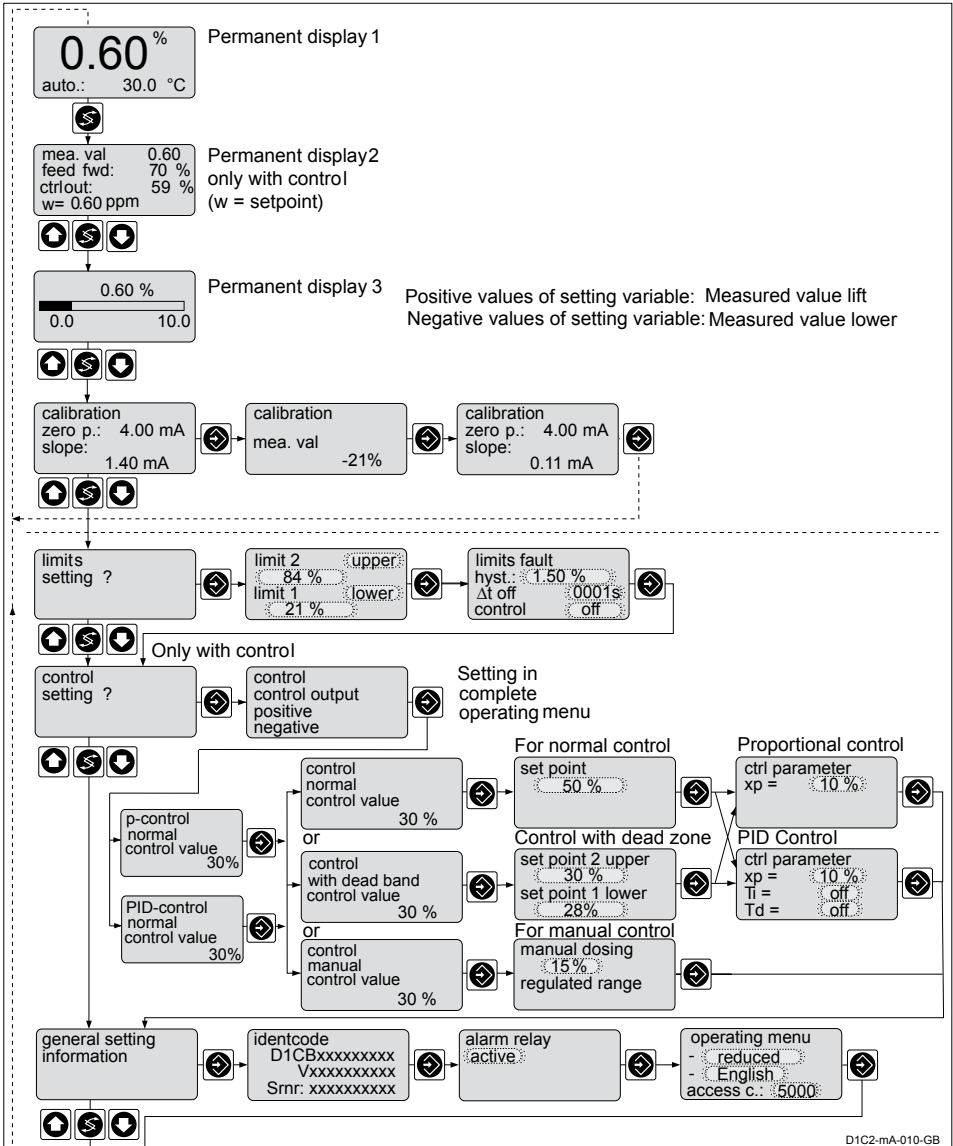


Fig. 51: Reduced operating menu / Shown with measured variable % and the measuring range 0%....100%

## 9.7 Complete Operating Menu / Description of All Measured Variables

The complete operating menu allows all control unit parameters to be set. The following overview shows the settings that can be selected:

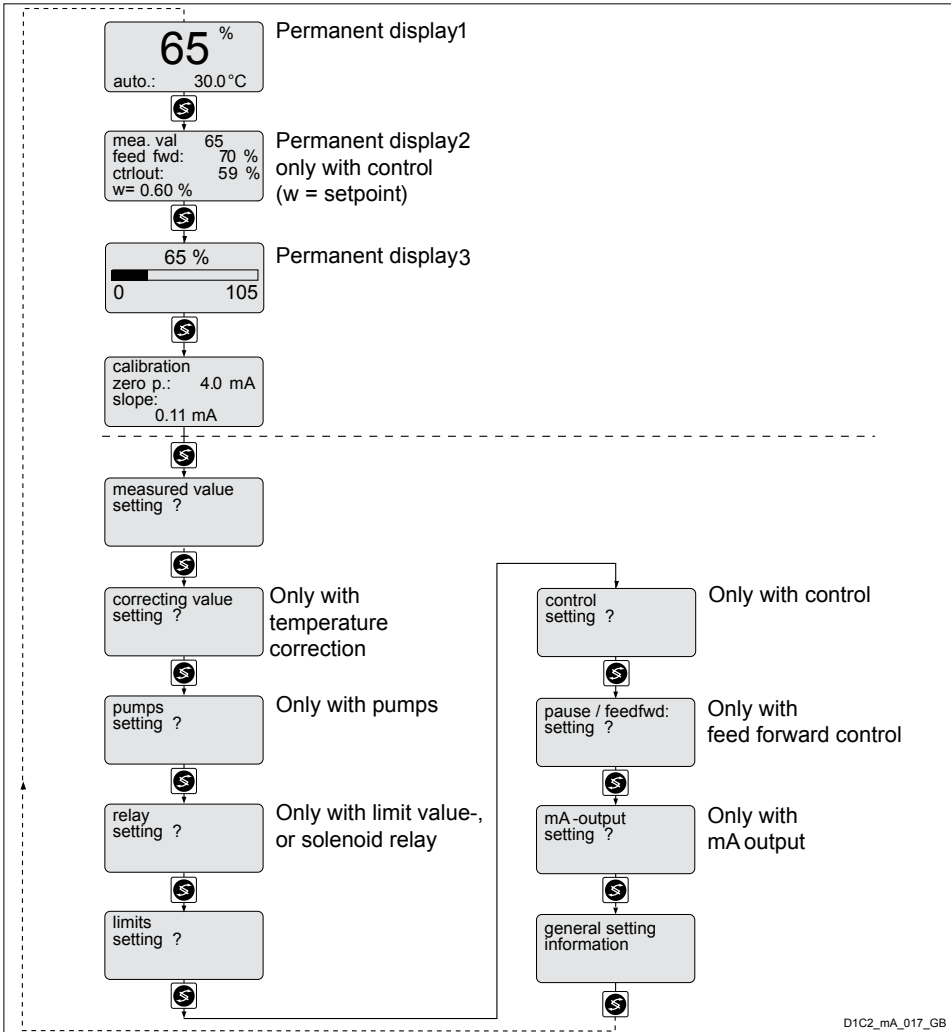


Fig. 52: Complete operating menu / Shown with measured variable % and the measuring range 0%.... 100%

### 9.8 Calibrating the Standard Signal

In the restricted operating menu: The DULCOMETER® D1Cb / D1Cc calibrates the zero point.

In the complete operating menu: The DULCOMETER® D1Cb / D1Cc carries out a two-point calibration.



#### **WARNING!**

##### **Incorrect metering due to incorrect metering range**

Possible consequence: Fatal or serious injuries

- **The measuring range of the sensor or the measuring device is essential for the measuring range!**
- If the assignment of the measuring range is modified, the settings must be checked in all menus
- If the assignment of the measuring range is changed, the sensor or the measuring device must be recalibrated



#### **CAUTION!**

##### **Correct sensor operation / Run-in time**

Damage to the product or its surroundings

- Correct measuring and dosing is only possible if the sensor is working perfectly
- Please read the operating manual for the sensor or the measuring device
- It is imperative that the run in periods of the sensors or the measuring device are adhered to
- The run in periods should be allowed for when planning commissioning
- It may take a whole working day to run-in the sensor or the measuring device

## Measured Variables and Operating Menus for the Standard Signal General

During the calibration, the DULCOMETER® D1Cb / D1Cc sets the control outputs to "0". Exception: a basic load or a manual control value has been set. This remains active. The mA standard signal outputs are frozen. The measured value frozen at the start of calibration is suggested as a value. This value can be set using the arrow keys. Calibration is only possible if the value is  $\geq 2\%$  of the measuring range of the sensor or the measuring device.

### Error messages in the calibration menu

Fault message	Condition	Effect
Measured value gap too small	$\Delta$ value $< 5.0\%$ *	Measured value is rejected;
	$\Delta$ value $< 1.00\text{ mA}$ *	Repeat calibration of the measuring point!

Refer to the operating manual of the respective sensor for all error messages and use for troubleshooting.

\* of the measuring range and measured value, see ↗ *Table on page 105*

### 9.8.1 Calibration of the Zero Point of the Standard Signal General

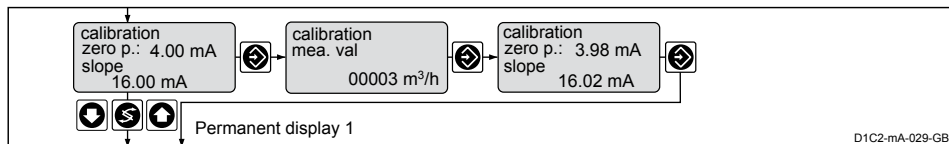










Fig. 53: Zero point calibration menu / shown with flow as the measured variable and the measuring range 0...100 m<sup>3</sup>/h



The slope in the calibration menu is given as an mA value. This value should be regarded as the mA/selected measuring unit.

## Calibration in the restricted operating menu

1. ▶ Select the calibration menu. Then press 
2. ▶ Enter the actual value suitable for the respective measured variable determined using the measuring method with the keys ,  and  in the DULCOMETER® D1Cb / D1Cc. Confirm entry with the key 
3. ▶ Continue with . Should an error be displayed, see  'Error messages in the calibration menu' Table on page 110
  - ⇒ Calibration is completed.
4. ▶ Continue with 
  - ⇒ The display now shows the values determined for the zero point and slope.

## 9.8.2 Two-Point Calibration of the Standard Signal General












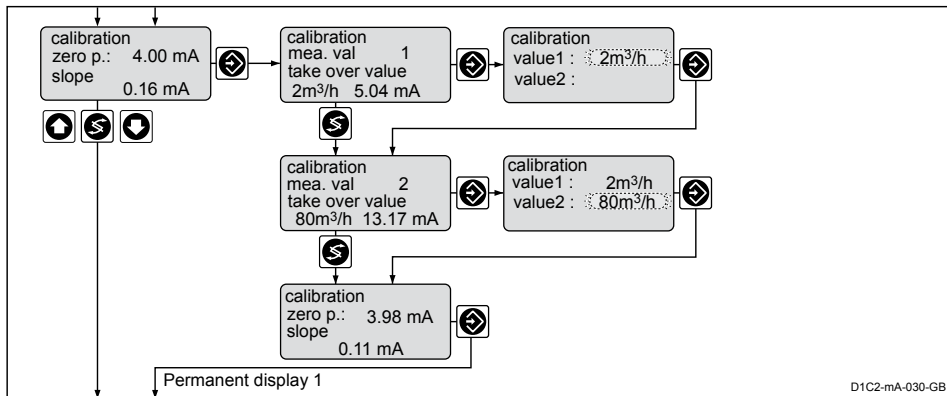





Fig. 54: Two point calibration menu / shown with flow as the measured variable and the measuring range 0... 100 m<sup>3</sup>/h

### Calibration in the complete operating menu

1. ➤ Select the calibration menu. Then press 
2. ➤ Confirm prompt with the key 
3. ➤ Enter the actual value 1 suitable for the respective measured variable determined using the measuring method with the keys ,  and  in the DULCOMETER® D1Cb / D1Cc. Confirm entry with the key . The value flashes
4. ➤ Continue with 
5. ➤ Confirm prompt with the key 
6. ➤ Enter the actual value 2 suitable for the respective measured variable determined using the measuring method with the keys ,  and  in the DULCOMETER® D1Cb / D1Cc. Confirm entry with the key . The value flashes
7. ➤ Continue with 
  - ⇒ The display now shows the values determined for the zero point and slope. Should an error be displayed, see  'Error messages in the calibration menu' Table on page 110



## 10 Operating Menus Independent of Measured Variables

- **Users' qualification:** instructed persons, see ↗ *Chapter 1.2 'Users' qualifications' on page 10*



### ***Operating Menus Independent of Measured Variables***

*This section describes of the DULCOMETER® D1Cb / D1Cc operating instructions describes the operating menus, which are independent of the measured variable.*

### 10.1 Pumps

#### CAUTION!

##### Observe the operating manual for the pump

Possibility of damage to the pump. Faults in the process.

- The pump must be set to "External Control" operating mode
- Observe the maximum stroke rate for the pump
- Possibly switch off any stroke memories in the pump controller
- The maximum stroke rate for the pump can be found in the operating manual for the pump
  - Setting a stroke rate on the controller, which is higher than the actual possible maximum stroke rate of the pump, can lead to hazardous operating conditions

#### NOTICE!

##### Maximum pump frequency

The pumps are activated in accordance with the actuating variable up to the respective maximum frequency of the pump.

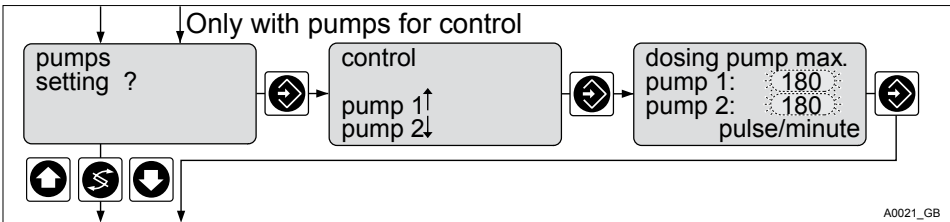


Fig. 55: Pumps

---

## Operating Menus Independent of Measured Variables

---

	Factory setting	Possible values			Remarks
		Increment	Lower value	Upper value	
Strokes	180	1	0	500	
<b>Critical when setting the stroke rate is the flow rate of the pump in relation to the respective process. Observe the maximum pump frequency</b>					

### 10.2 Setting the Relays



#### **Relay combination**

*Relay 1 and relay 2 can be configured independently of each other. Thus any combination of "Off / Limit / Actuator / SV / Timer" is possible.*

		Possible values			
	Factory setting	Increment	Lower value	Upper value	Remarks
Relay assignment	As per identity code	Solenoid valve (SV1, SV2) Limit value (limit 1/2)* Actuator 1/2 Timer 1/2 Off			*At the limit, the relays remain activated even in the event of a malfunction.
Cycle	10 s	1 s	10 s	9999 s	For solenoid valve
Min. time	1 s	1 s	1 s	Cycle/2	For solenoid valves: the smallest permissible switch-on period of the connected device should be set here
Cycle	Off	1 h	1 h/off	240 h	For timer
T On	1 minute	1 minute	1 minute	240 min.	For timer

## 10.2.1 Setting and Functional Description of the Relays

### 10.2.1.1 Setting and Functional Description of "Relay Off"

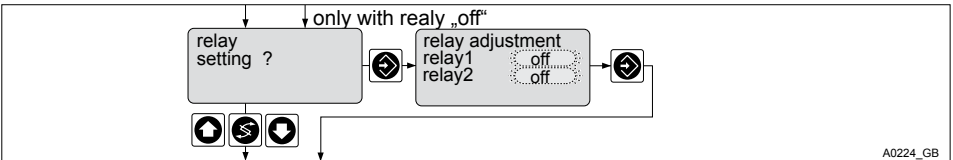


Fig. 56: Relay off

The functionality of the relays is switched off.

### 10.2.1.2 Setting and Functional Description of "Relay Used as a Limit Relay"

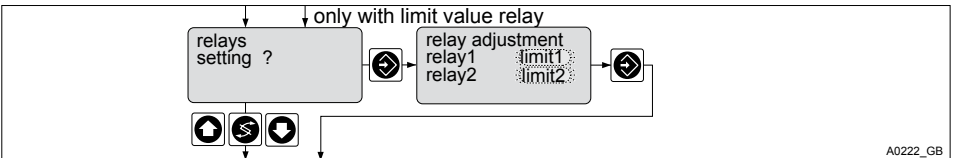


Fig. 57: Limit relay

Relay 1 and/or relay 2 can be configured as limit relays. The limit values can be set in the menu [Chapter 10.3 'Setting the Limits' on page 122](#).

### 10.2.1.3 Setting and Functional Description of "Relay Used as an Actuator"

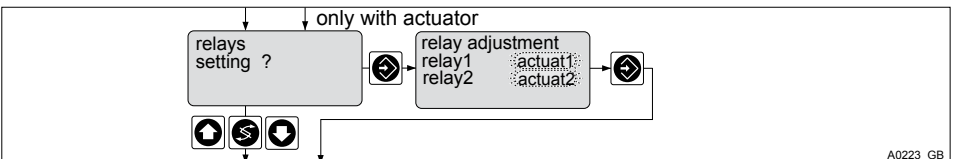


Fig. 58: Relay used as an actuator

### **Limit relay used as an actuator**

#### Extended functions

- The limit relays can also be defined in such a way that they react like an actuator. If, for example, a limit relay is activated, then it is deactivated if the pause contact is closed and for a subsequent time delay  $t_d$  (if  $t_d > 0$  min is set under "General Settings").

### 10.2.1.4 Setting and Functional Description of the Timer Relay

#### **CAUTION!**

**The timer is reset when there is no supply voltage**

Possible consequence: slight or minor injuries. Material damage.

- Configure the power supply in such a way that it cannot be interrupted
- With critical processes, the possible failure of the timer should be practically addressed

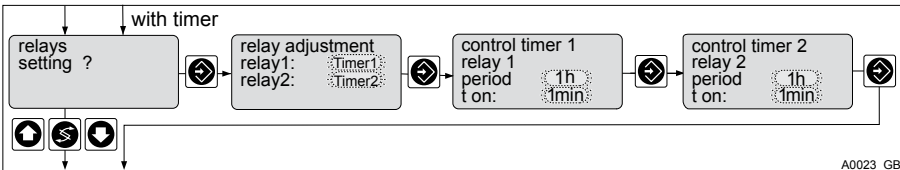


Fig. 59: Timer relay

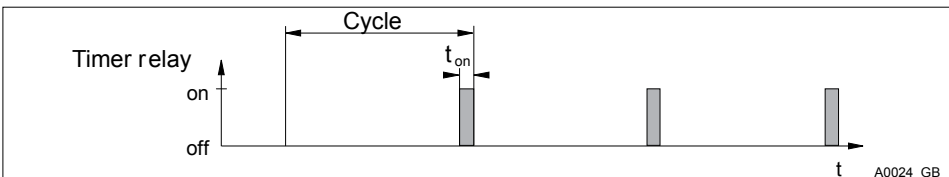


Fig. 60: Timer relay

At the end of the (Timer) cycle time, the DULCOMETER® D1Cb / D1Cc closes the corresponding timer relay for the duration of "t on" (Timer). "Pause" interrupts the timer. If the clock is visible on the LCD display, then the timer can be reset to the beginning of the cycle using the enter key. The % specification on the LCD display indicates the remaining runtime.

## 10.2.1.5 Setting and functional description of "Relay Used as a Solenoid Valve"

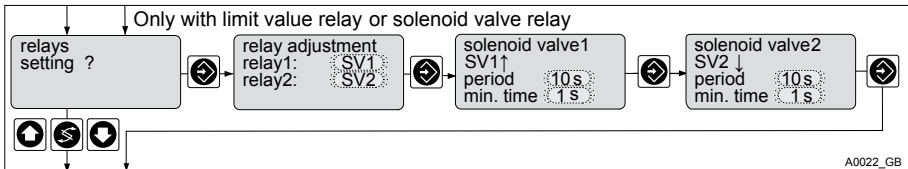


Fig. 61: Solenoid valve relay

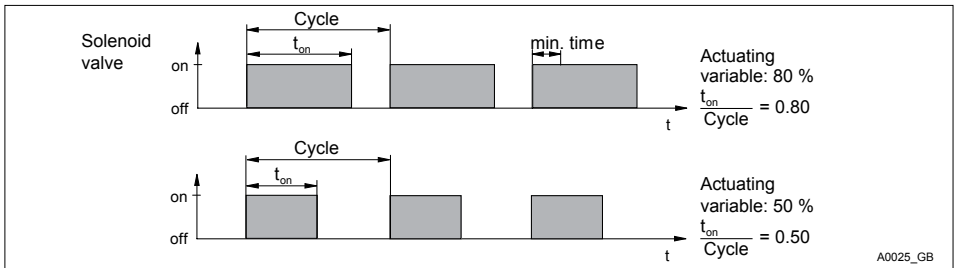


Fig. 62: Solenoid valves

The switching times of the relay (solenoid valve) depend on the control value and on the "minimum time" (smallest permissible switching time of the connected device). The control value determines the ratio  $t_{on}/cycle$  and thus also the switching times.

### 10.2.1.5.1 Switching Times of the Solenoid Valves

The switching times of the DULCOM-ETER® D1Cb / D1Cc (solenoid valve) depend on the cycle time and the "minimum time" (smallest permissible switching time of the connected device). The control value determines the ratio  $t_{on}/$  cycle and thus also the switching times. The "min. time" affects the switching times in two situations:



## First theoretical switching time < min. time

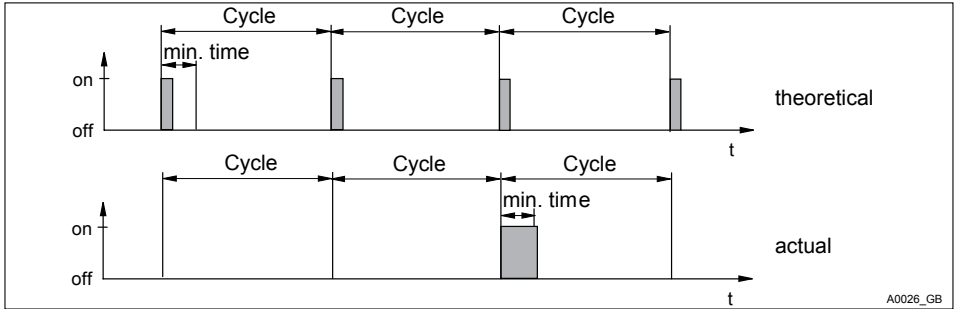


Fig. 63: Theoretical switching time < min. time

The DULCOMETER® D1Cb / D1Cc does not switch on for a certain number of cycles until the sum of the theoretical switching times exceeds the "min. time". Then it switches for the duration of this total time.

## Second theoretical switching time > (cycle - min. time):

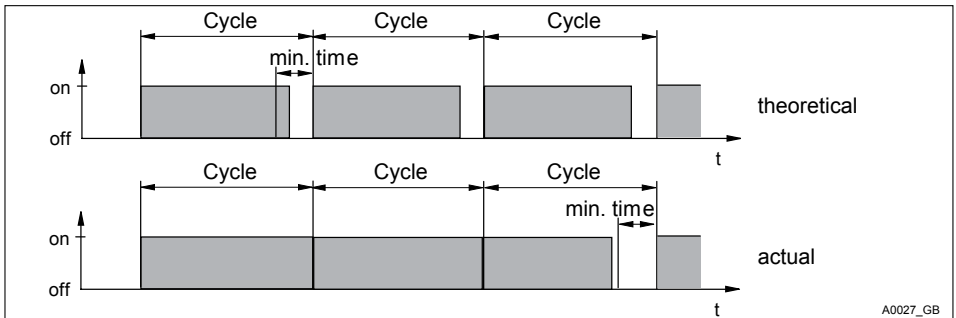


Fig. 64: Theoretical switching time > (cycle - min. time) and calculated switching time < cycle

The DULCOMETER® D1Cb / D1Cc does not switch off for a certain number of cycles until the differences between the cycle and the theoretical switching time exceed the "min. time".

## 10.3 Setting the Limits

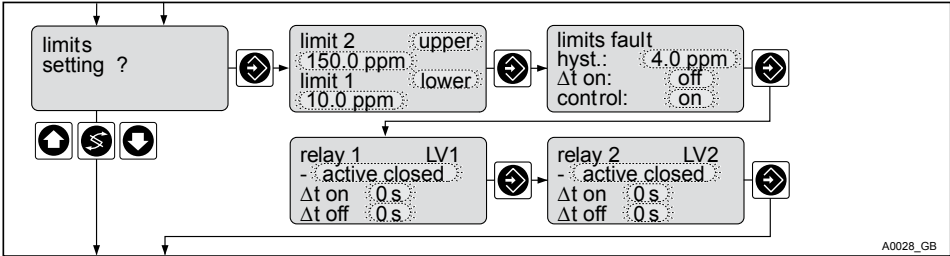


Fig. 65: Limits

The lower display row in the diagram A0028 is only visible if the relays have been defined as limit relays or as actuators in the menu *Chapter 10.2 'Setting the Relays'* on page 116.

### Setting options in the "Set Limit Values" menu

		Possible values			
	Factory setting	Increment	Lower value	Upper value	Remarks
Type of limit transgression					Limit transgression by exceeding or dropping below limits
Limit 1	Lower	Lower / Upper / Off	Lower	Upper	
Limit 2	Upper				
Limit value Limit 1	20 %	1 %		Upper limit of measured value	Effective in the direction of cancelling limit transgression
Limit value Limit 2	80 %	1 %			
Hysteresis limit	2 %	1 %			

## Operating Menus Independent of Measured Variables

	Factory setting	Possible values			Remarks
		Increment	Lower value	Upper value	
Checkout time limits $\Delta t$ on	Off	1 s	1 s	9999 s	Results in message and alarm, Off = 0 s, function switched off No message, no alarm
Control	On	On Off			
Limit value 1 (GW1)	Active closed	Active closed / Active open			Acts as N/O
Limit value 2 (GW2)	Active closed				
Switch-on delay $\Delta t$ on	0 s	1 s	0 s	9999 s	0 s = off

If the limit is exceeded for longer than the "Checkout time limits ( $\Delta t$  on)", then a fault message will be triggered that has to be acknowledged and the alarm relay is deactivated. If the "controller" is also set to "Off" then the control process is stopped.

"Lower limit" means that the limit criterion has been undercut.

"Upper limit" means that the limit criterion has been exceeded.

The DULCOMETER® D1Cb / D1Cc has an option for defining "Hysteresis limits".

The "hysteresis" works towards rectifying the limit transgression, i.e. if the "limit 1 upper" of, for example, pH 7.5 has been exceeded at a set hysteresis limit of, for example, pH 0.20, then the criterion for limit transgression is redundant when the value drops below the lower limit of pH 7.3. The hysteresis behaviour for a "lower limit" functions in a similar way (the hysteresis value is added to the limit). In this way it is possible to forego an external relay in self-retaining mode.

If the limit is exceeded for longer than the "Delay period limits  $\Delta t$  on", then an acknowledgeable fault message will be triggered and the alarm relay is deactivated. If the "controller" is also set to "Off" then the control process is stopped.

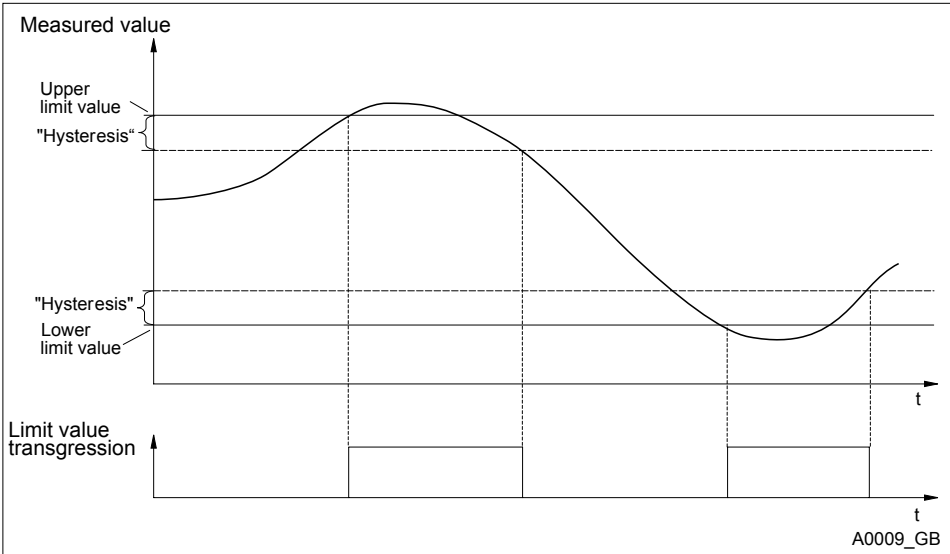


Fig. 66: Hysteresis

If the relays are defined as limit relays, they will also switch to the alarm relay when a limit is transgressed and the direction of the limit transgression will be shown on the display by the symbols **↑** or **↓**.

Different on-delays ( $\Delta t$  On) and fall-delays ( $\Delta t$  Off) can be set for the limit relays for limit 1 and limit 2. These prevent the limit relay from switching back and forward if the limit is only exceeded for a short time (damping function).

If there are no limit relays, the limits can nevertheless be entered. The DULCOMETER® D1Cb / D1Cc shows the reactions described when a limit is transgressed

### Limit relay used as an actuator

If the relays are defined as actuators, then they react like actuating outputs. Example: in the event of Pause being activated or in the event of an alarm, an activated limit relay will be deactivated.

### 10.4 Setting the Control

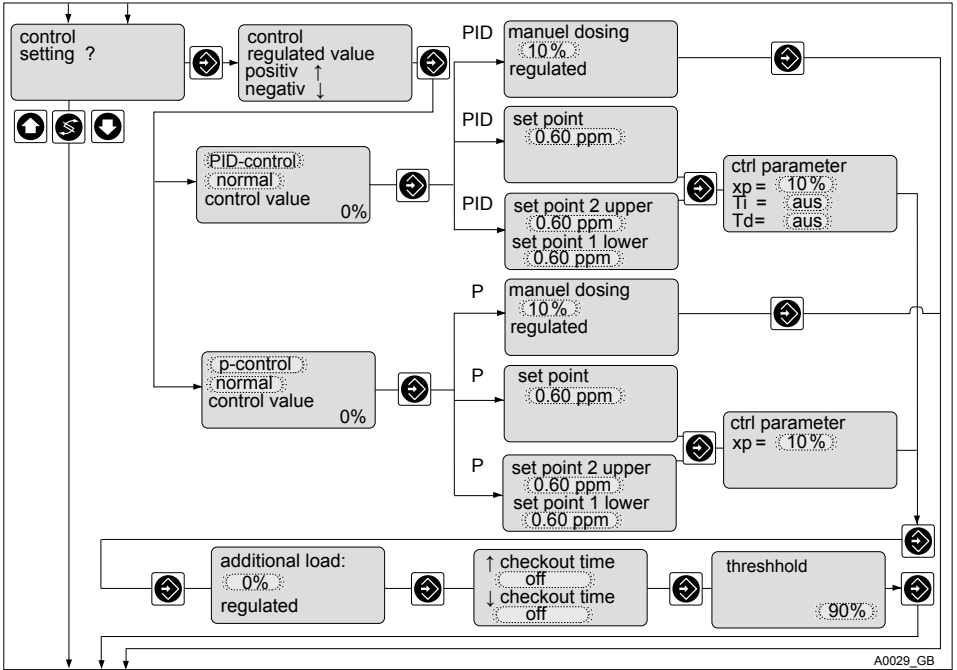


Fig. 67: Control

## Operating Menus Independent of Measured Variables

With control with a dead zone, the control variable does not change with measured values within the dead zone. The setting ranges are specified by the DULCOMETER® D1Cb / D1Cc.

### Setting values of the control

		Possible values			
	Factory setting	Increment	Lower value	Upper value	Remarks
Control	normal	normal with dead zone Manual			With control with a dead zone, only the additive basic load is given as the control variable for measured values within the dead zone
Setpoint	0.5 * measuring range	depending on the measured variable and measuring range	lower limit of measuring range	Upper limit of measuring range	During control with a dead band, 2 setpoints are necessary. Setpoint 1 > setpoint 2
Control parameter xp	10 % of the measuring range	depending on the measured variable and measuring range	1 % of the measuring range	120 % of the measuring range	
Control parameter Tn	off	1 s	1 s	9999 s	Function off = 0 s

	Factory setting	Possible values			Remarks
		Increment	Lower value	Upper value	
Control parameter Tv	off	1 s	1 s	2500 s	Function off = 0 s
Additive basic load	0 %	1 %	-100 %	+100 %	
Manual dosing	0 %	1 %	- 100 %	+100 %	
↑ checkout time	off	1 min	1 min	999 min	
↑ checkout time	off	1 min	1 min	999 min	
Threshold	90 %	1 %	0 %	100 %	

**Declaration: What effect do checkout time and threshold have?**

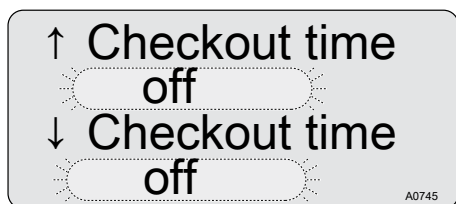


Fig. 68: checkout time

The *[checkout time]* of the control should prevent over dosing with chemicals in the event of a fault.

Example: Sample water flows past the sensor in such a way that in spite of dosing, no chemicals reach the sensor. The sensor cannot detect any change in the measured value. There are now enough chemicals in the sample water but the controller continues dosing because it

does not detect any change in the measured value. Here the *[checkout time]* protects the control process. The controller stops the control and thus also the dosing of chemicals.

Control is stopped if during a settable time (= *[checkout time]*) the control value lies above a control value threshold (= *[threshold]*). The *[checkout time]* can be set differently for the control directions *[raise ↑]* and *[lower ↓]*. This makes sensor for a two-sided pH control, if the concentration of the acids and alkalis are different.

# threshold

90%

A0746

Fig. 69: Threshold

The maximum permitted control value [*Threshold*] must be set = maximum allowed control value.



### **The control of your process**

*The values for [checkout time] and [threshold] depend on the process, in which the measurement and control are taking place. These values can be very individual and depend on many factors (such as the chemicals used etc.). Hence we cannot specify any values for you. You will have to determine these values for yourselves.*

Before you can specify the [*checkout times*] and [*threshold*], you must monitor the control of your process over a representative period and determine the necessary dosing times and control values.

You must select the [*checkout times*] and the [*threshold*] so that in normal operation they are not exceeded. If the [*checkout time*] of the control is transgressed, the control is stopped and an error message is displayed. You must acknowledge this error message to restart the control.



### **Transgression of the checkout time**

*If a transgression of the [checkout time] repeatedly occurs, then you must clear the error in the process or redetermine and reset the values for the [checkout times] and the [threshold].*

1. Acknowledge the error message with the [*Enter*] key
2. Reset the controller into normal operation using the [*Start/Stop*] key



### 10.5 Set mA output

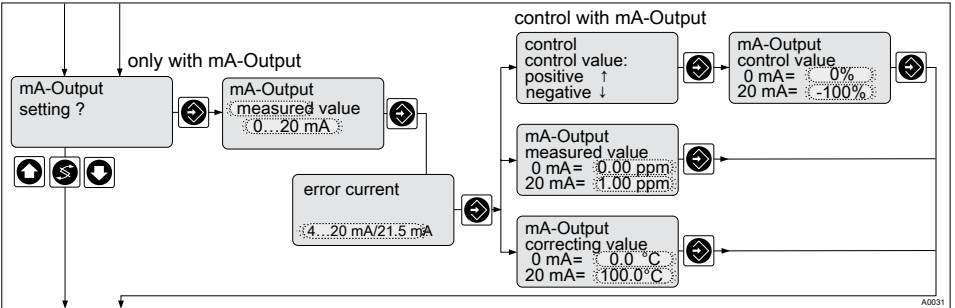


Fig. 70: mA-Output

### Set values of the mA-Output

	Factory setting	Possible values			Remarks
		Increment	Lower value	Upper value	
Assignment of variable	Off	Measured value			
		Control value			Possible if control available
		Correcting value			Only available with correction variable
		Off			
Range	0 – 20 mA	0-20 mA			
		4-20 mA			
		3.6/4-20 mA			Reduction to 3.6 mA if alarm relay is switched

## Operating Menus Independent of Measured Variables

	Factory setting	Possible values			Remarks
		Increment	Lower value	Upper value	
Measured value range	0 ppm ...max. Measuring range	0.01 ppm	0 ppm	Upper limit of measuring range	Minimum range 0.1 ppm
	- 1 pH...max. Measuring range	0.01 pH	-1 pH		
	0 mV...max. Measuring range	1 mV	- 1200 mV		
	0.0 °C...max. Measuring range	0.1 °C	0.0 °C		
	mA	0.01 mA	- 1 mA		
Control variable range	-100 % - 0 %	1 %	-100 %	100%	Minimum range 1 %
Correction value range	0 – 100 °C	0.1 °C	0 °C	100 °C	Minimum range 1 °C
Fault current	4...20mA/ 21,5mA	off 3.6/4 ... 20 mA 4...20mA/ 21,5mA			

## 10.6 General settings

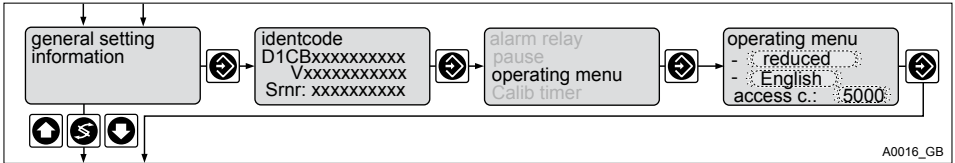


Fig. 71: General settings

The functions described below can be selected in this menu.

### 10.6.1 Setting the Measured Variable/Measuring Range



#### WARNING!

#### Incorrect metering due to incorrect metering range

Possible consequence: Fatal or very serious injuries

- If the assignment of the measuring range is modified, the settings must be checked in all menus
- If the assignment of the measuring range is changed, the sensor or the measuring device must be recalibrated
- The measuring range of the sensor or the measuring device is essential for the measuring range!

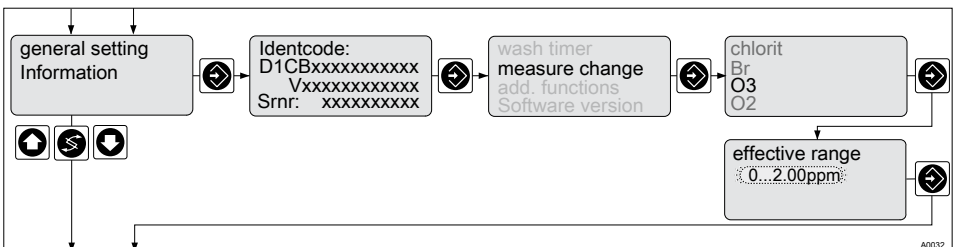


Fig. 72: Measuring range

In the "Change measured variable" setting range, it is possible to select the measured variable required for the respective process and suitable for the sensor or measuring device. Depending on the measured variable, different setting windows must be processed, which are provided by the software of the DULCOMETER® D1Cb / D1Cc. The values are set, selected and confirmed using keys , , and .

### 10.6.2 Sub-Functions of the "General Settings" Menu

The following sub-functions can be found in the "General Settings" menu item.

#### 10.6.2.1 Operating Menu



In the "Operating Menu" menu item, the language in which the operating menu is displayed can be selected and it is also possible to select between a "reduced" and "complete" operating menu.

#### 10.6.2.2 Calibration Timer

The calibration timer reminds the user of a routinely necessary calibration. The calibration timer is activated by inputting a number of days. Recalibration is necessary at the end of this period.

The calibration timer serves to remind the device operator that the connected sensors need to be recalibrated. The time is thus not based directly on the state of the sensors but on the expiry of a period of time set by the operator. If the calibration timer is enabled, an interval of between 1 and 100 days can be entered. If the calibration timer is activated and if the menu is called up again, the remaining period of time until the timer runs out is shown by way of information. A remaining time of less than one day is shown in "hours".

Resetting the timer: The calibration timer is automatically reset to its initial value following a successful calibration. Any possible display message disappears.

"Snooze" mode: If the calibration timer has expired, the message on the display can be acknowledged for a period of 15 minutes by pressing the  button. The message "Calibration timer" will reappear. The  key has to be pressed for as long


as the "Calibration timer" message is visible. If another message is shown alternately, it is necessary to wait until the "Calibration timer" message reappears. Any fault messages have priority.


#### 10.6.2.3 Wash Timer

The wash timer is used to remind the operator of the DULCOMETER® D1Cb / D1Cc than cleaning of the connected sensors is necessary. The time is thus not based directly on the state of the sensors but on the expiry of a period of time set by the operator.

The "Wash timer" entry can be found in the system menu. The washing timer can be enabled and disabled in this menu. If the washing timer is enabled, an interval of between 1 and 100 days can be entered. If the washing timer is enabled and if the menu is called up again, the remaining period of time until the timer runs out is shown for information. A remaining time of less than one day is shown in "hours".

Resetting the timer: once the washing timer period has expired, it can be reset in the associated menu.

"Snooze" mode: If the wash timer has expired, the message on the display can be acknowledged for a period of 15 minutes by pressing the  key. The message "Wash timer" will then reappear.

Pressing the  key must be carried out for as long as the "Wash timer" message is visible. If another message is shown alternately, it is necessary to wait until the "Wash timer" message reappears. Any fault messages have priority.

### 10.6.2.4 Change Measured Variable

#### Change Measured Variable

In the "Change Measured Variable" menu item are listed all of the measured variables which can be enabled by the enabling code. ↪ *Chapter 10.6.1 'Setting the Measured Variable/Measuring Range' on page 131*

### 10.6.2.5 Additional Functions

In the "Additional Functions" menu item, the range of functions of the DULCOMETER® D1Cb / D1Cc can be changed by inputting an optionally available enabling code. ↪ *'Extended functions' on page 55*

### 10.6.2.6 Operating hour counter

The DULCOMETER® D1Cb / D1Cc has resettable operating time counter.

"Operating hours" menu item: The operating hour counter has a resolution of one minute and a maximum fault in the event of power failure of 5 minutes. The operating hour counter cannot be reset.

### 10.6.2.7 Calibration Logbook

The data on the successfully completed sensor calibrations are stored in the internal calibration logbook. Up to 30 calibrations can be stored. Thereafter the oldest entry is overwritten with the most recent entry.

The following data is stored:

- Time of calibration (as per the operating hour counter)

- d = day
- h = hour
- m = minute

- Zero point (without unit)
- Gradient (without unit)

### 10.6.2.8 Software Version

The version of the software currently installed and the hardware revision are shown under the menu item *[Software version]* for the DULCOMETER® D1Cb / D1Cc.

### 10.6.2.9 Alarm Relay

The alarm relay signals, together with the **E** and an error message, that there is an error. This may consist of a:

- General device error
- Power failure: The relay is activated if voltage is supplied to the control unit and there is no error. If the voltage is disconnected, then the relay is deactivated
- Upper and lower limits of measuring range breached
- Limit transgression, even without limit relay, if the control time is set to "Limit value > 0 s" and is exceeded
- Sensor failure with pH (short circuit or no sensor connected)
- Overload/short circuit at mA sensor input
- If alarm relay "active" has been selected in the "Pause" menu item and pause is active

### 10.6.2.10 Sensor Monitoring (pH Sensor mV Only)

With configured pH measured variables, it is possible to monitor a sensor connected to the potentiometric input for fault states. This check is disabled as standard.

Monitoring for sensor breakage: The sensor breakage check (broken probe) can identify a defective sensor by means of its low internal resistance. Correctly functioning pH sensors have very high resistances with internal resistances in the high M $\Omega$  range. The DULCOMETER® D1Cb / D1Cc is capable of recognising broken sensors from their internal resistance. This function should be deactivated if very low resistance sensors are used.

Refer also to:  Table on page 146

Check for presence: The "Check for availability" identifies a disconnected sensor or a broken cable. This function should be disabled if pH sensors are used, which have a high internal resistance across their entire operating range.

### 10.6.2.11 Pause

#### "Normal" Pause function

If the pause contact is closed, the controller sets the control outputs to '0', as long as the pause contact is closed or for a subsequent delay period 'td' (if a min. 'td > 0' is set). While the Pause contact is closed, the controller records the 'P' term in the background.

#### PID control

*An I term is generally only present if, in the setting menu 'set control?' 'Tn > 0' has been set.*

*Exception: The mA-Outputs for the measured value or correcting value are unaffected by the Pause.*

For PID control: An I term present when closing the Pause contact is saved. Once the Pause contact has been opened, the control outputs 'td' remain '0' for the length of the delay period. The delay period 'td' must be set in such a way that, for example, during this period the sample water, which contains sufficient feed chemical (e.g. chlorine), for the typical process, flows to the sensor.

For PID control: The control variable issued following the Pause and the expiry of the delay period 'td' consists of the current P term and ('Tn > 0') the stored I term.

#### "Hold" Pause function

If the pause contact is closed, the controller sets the control outputs to the last value, as long as the pause contact is closed or for a subsequent delay period 'td' (if a min. 'td > 0' is set).

While the Pause contact is closed, the controller records the P term in the background.

For PID control: The standard mA signal outputs (measured value or correcting value) are also frozen. After the Pause contact has been opened, the control output remain frozen for the delay period 'td'. The delay period 'td' must

be set in such a way that, for example, during this period the sample water, which contains sufficient feed chemical (e.g. chlorine), for the typical process, flows to the sensor.

For PID control: The control value issued following the Pause and the expiry of the delay period '  $t_d$  ' consists of the current P term and (if '  $Tn > 0$  ' is set) the newly determined I term.

### 10.6.2.12 Temperature

In the "Temperature" menu item, the unit in which the temperature is displayed can be switched between °C and °F.

# 11 Maintenance

- **Users' qualification:** trained user, see ☞ *Chapter 1.2 'Users' qualifications' on page 10*

The DULCOMETER® D1Cb / D1Cc is maintenance free.

## 11.1 Fuse replacement DULCOMETER® D1Cb / D1Cc



### WARNING!

#### Danger from electrical voltage

Possible consequence: Fatal or very serious injuries.

- The DULCOMETER® D1Cb / D1Cc does not have a mains switch
- When working inside the controller, disconnect the controller from the mains power via an external switch or by removing the external fuse



### WARNING!

#### Danger from electrical voltage

Possible consequence: Fatal or very serious injuries.

- There may still be mains voltage on terminals XR 1 - 3 even after disconnection of the power supply
- These can be separately supplied externally with mains voltage
- Terminals XR 1 - 3 should be disconnected separately from the mains voltage



### NOTICE!

#### Use only 5 x 20 mm micro-fuses

Possible consequence: Damage to the product or its surroundings

- 100 – 240 V ☞ *Table on page 148*



### **Fuse change**

The mains fuse is located in a sealed fuse holder inside of the device, see Fig. 10.

- 1.** ▶ Disconnect the controller from the mains power
- 2.** ▶ Open the controller and put the upper section of the housing into its "parked position"
- 3.** ▶ Remove cap of micro-fuse
- 4.** ▶ Remove the micro-fuse using a suitable tool
- 5.** ▶ Fit the micro-fuse using a suitable tool
- 6.** ▶ Fit cap of micro-fuse
- 7.** ▶ Replace upper section of housing and close the controller

## 11.2 Summary of Error Texts

Error	Error text	Symbol	Effect on actuating variable	Effect on control	Alarm with acknowledgement	Remarks
Actuating variable exceeds control time of reading	Check sensor	Ξ	Basic load	Stop	Yes	Function can be switched off
Upper and lower limits of signal breached  (only with mA input)	Input	Ξ	Basic load	Stop	Yes	Signal <math>3.0 \pm 0.2 \text{ mA}</math> or >math>23 \pm 0.2 \text{ mA}</math>
Calibration sensor has a fault	Compensation defective	Ξ	Basic load	Stop	No	Metering continues with fault with unsteady readings

Error	Error text	Symbol	Effect on actuating variable	Effect on control	Alarm with acknowledgement	Remarks
Correction variable - upper/lower signal breached	Temp. input	Ξ	Basic load	Stop	Yes	Pt100 signal >138.5 Ω signal, <100 Ω  Pt1000 signal >1385 Ω signal, <1000 Ω  The last valid value will be reused
Limit value transgression after control time of limit value	Limit value 1	Ξ	Stop or basic load	Stop	Yes	Function can be switched off
	Limit value 2	Ξ			Yes	

Operating step	Message text	Symbol	Effect on actuating variable	Effect on control	Alarm with acknowledgement	Remarks
Pause contact	Pause	Ξ ΞO	Stop	Stop	No/Yes*	No further error check
	Pause/ Hold	Ξ		PI frozen		
Stop key	Stop	Ξ ΞO	Stop	Stop	No	Relays drop out

## Maintenance

Operating step	Message text	Symbol	Effect on actuating variable	Effect on control	Alarm with acknowledgement	Remarks
During calibration of sensors			Basic load		No	No error treatment of measured variable
Sensor gradient too low		⊗	Basic load		No	25% > sensor gradient
Sensor gradient too high		⊗	Basic load		No	> 300% of standard gradient
DPD < 2 % of measuring range	DPD value too small					
Zero point	Zero point low Zero point high	⊗				Signal < 3 mA Signal > 5 mA

\*Dependent on whether "Alarm Off" or "Alarm On" is set in "General Settings"

## 12 Technical data

### 12.1 Ambient conditions DULCOMETER® D1Cb / D1Cc

#### Permissible ambient conditions:

Wall mounted:	0° C – 50° C
Control panel installation:	0° C – 50° C
All versions:	10 to 95% relative air humidity (non-condensing)

#### Permissible storage conditions:

All versions:	-10° C – 60° C
All versions:	< 95% relative air humidity (non-condensing)

### 12.2 Sound Pressure Level

No noise generation measurable

### 12.3 Material Data

<b>Part</b>	<b>Material</b>
Housing lower and upper section	PPE-GF10
Bracket on rear of housing lower section	PPE-GF20
Membrane keypad	Polyester PET membrane
Seal	CR foam rubber
Angle bracket and screws	Galvanically galvanised steel
M5 screws	Stainless steel A2

### 12.4 Chemical Resistance

The device is resistant to normal atmospheres in plant rooms

## 12.5 Dimensions and weights

### D1Cb

Complete device:	198 x 200 x 76 mm (W x H x D)
Packaging:	390 x 295 x 155 mm (W x H x D)
Weight of device without packaging:	approx. 1.2 kg
Gross weight of device with packaging:	approx. 2.0 kg

### D1Cc

Complete device:	96 x 96 x 140 mm (W x H x D)
Packaging:	390 x 295 x 155 mm (W x H x D)
Weight of device without packaging:	approx. 1.2 kg
Gross weight of device with packaging:	approx. 2.0 kg

---

## Electrical Data

---

### 13 Electrical Data

Mains connection	
Nominal voltage range:	100 – 230 VAC $\pm$ 10 %
Frequency	50 – 60 Hz
Current consumption	95 – 250 mA

The mains connection is isolated from other switching parts by reinforced insulation. The device has no mains switch; a fuse is fitted.

Power relay	
Loading of switching contacts:	5 A; no inductive loads
	Use protective RC circuit (optional) with inductive loads

Alarm Relay	
Loading of switching contacts:	5 A; no inductive loads
	Use protective RC circuit (optional) with inductive loads

Outputs galvanically isolated from other switching parts by reinforced insulation.

Digital input	
Open circuit voltage:	6 V DC max.
Short circuit current:	approx. 0.6 mA
Max. switching frequency:	500 Hz at 50% filling factor



**! NOTICE!**

Do not supply with voltage

For the connection of an external semi-conductor or mechanical switch.

<b>mA Output</b>	
Current range:	0/3.8 – 23 mA
In the event of a fault:	3.6 or 21.5 mA
Max. apparent ohmic resistance:	450 $\Omega$ at 20.5 mA
Max. output voltage:	18 V DC
Overvoltage-resistant up to:	$\pm$ 30 V
Output accuracy:	$\pm$ 0.25 % of range

Galvanically isolated from all other connections (500 V)

<b>Pump activation</b>	
Max. switching voltage:	50 V (protective low voltage)
Max. switching current:	50 mA
Max. residual current (open):	10 $\mu$ A
Max. resistance (closed):	60 $\Omega$
Max. switching frequency (HW) at 50% filling factor	500 Hz

---

## Electrical Data

---

2 digital outputs isolated galvanically from each other and from all other connections via OptoMos relays.

mA Input	
Current measuring range	0...24 mA
Voltage output for passive transmitters:	approx. 21 V/max. 35 mA/ Ri min. 50 $\Omega$
Measuring accuracy:	$\pm 0.25$ % of range up to 22 mA *
Overvoltage-resistant up to:	$\pm 50$ V
Short circuit-resistant	Yes

\* Values above 22 mA only have an informative character

For the connection of active and passive power transmitters in 2- and 3-wire systems. Not galvanically isolated from the temperature and mV inputs.

Do not connect mV input and mA input simultaneously. Values will be falsified and the sensors and measuring devices connected will be damaged.

Switch off supply and current measuring resistance in the event of a fault; reactivate cyclically by means of software.

mV Input	
Measuring range:	-1 V...+1 V
Measuring accuracy:	$\pm 0.25$ % of range
Sensor monitoring of input (low ohmic threshold) (can be switched off):	< approx. 500 k $\Omega$ (short circuit)
Sensor monitoring of input (high ohmic threshold) (can be switched off):	> approx. 1.2 G $\Omega$
Overvoltage-resistant up to:	$\pm 5$ V

For the connection of potentiometric sensors. Short circuit monitoring provided by software.

Do not connect mV and mA simultaneously. Values will be falsified.

Not galvanically isolated from the mA and temperature inputs. Terminal for the connection of an electrode for compensating for the potential of the measuring liquid

<b>Temperature input</b>	
Temperature measuring range:	0...100 °C
Measuring flow:	approx. 0.96 mA
Measuring accuracy:	± 0.5 % of measuring range
Overvoltage-resistant up to:	± 5 V
Short circuit-resistant	Yes

For the connection of Pt100 or Pt1000 temperature sensors in 2-wire systems. A switch is automatically made between Pt100 / Pt1000. Not galvanically isolated from the mA and mV inputs.

## 14 Spare parts and accessories DULCOMETER® D1Cb / D1Cc

### Spare parts and accessories DULCOMETER® D1Cb

<b>Spare parts</b>	<b>Part number</b>
Fine fuse 5x20 T 1.6A	732411
Threaded connection M12x1.5 compl. metric	1032245
Half screw connection compl. metric	1031506
Wall bracket	792713
Guard terminal top part	733389
D1C/D2C measured variable labels	1030506

<b>Accessories</b>	<b>Part number</b>
Control panel assembly set	792908
Protective RC Circuit retrofit kit for D1Cb	1034238
SN6 input retrofit kit	1036885

---

## Spare parts and accessories DULCOMETER® D1Cb / D1Cc

---

### Spare parts and accessories DULCOMETER® D1Cc

Spare parts	Part number
Fine fuse 5x20 T 1.6A	732411
Guard terminal top part	733389
D1C/D2C measured variable labels	1030506

Accessories	Part number
2 pole female multipoint connector for relays and power supply	731043
3 pole female multipoint connector for alarm relays	731044
8 pole female multipoint connector, black	733562
8 pole female multipoint connector, red	733563

### 15 Standards Complied With

DIN EN 61010 Safety requirements for electrical units for measuring, control, regulating and laboratory devices

DIN EN 61326 Electrical equipment for measuring, control and laboratory use - EMC requirements (for class A and B devices)

DIN EN 55014-1 EMC Requirements of household appliances Part 1 Emitted interference

DIN EN 55014-2 EMC Requirements of household appliances Part 2 Interference resistance

## 16 Disposal of Used Parts

- **Users' qualification:** instructed persons, see ↗ *Chapter 1.2 'Users' qualifications' on page 10*

### ! NOTICE!

#### Regulations governing disposal of used parts

- Note the current national regulations and legal standards which apply in your country

ProMinent Dosiertechnik GmbH, Heidelberg will take back decontaminated used devices providing that they are covered by adequate postage.

You can find the currently valid decontamination declaration for Download under [www.prominent.com](http://www.prominent.com).

### 17 Declaration of Conformity


EC Declaration of Conformity	
We,	ProMinent Dosiertechnik GmbH Im Schuhmachergewann 5 - 11 DE - 69123 Heidelberg
hereby declare that, the product specified in the following complies with the relevant basic health and safety rules of the EC Directive, on the basis of its functional concept and design and in the version marketed by us. This declaration loses its validity in the event of a modification to the product not agreed with us.	
Description of the product:	DULCOMETER Measuring and Control Device
Product type:	D1Cb ...
Serial no.:	refer to nameplate overleaf and on the device
Relevant EC Directives:	EC Low Voltage Directive (2006/95/EC) EC EMC Directive (2004/108/EC)
Harmonised standards applied, in particular:	EN 61010-1, EN 61326-1
Date / manufacturer's signature:	12.05.2009 
Details of the signatory:	Joachim Schall, Head of Development

Fig. 73: EC Declaration of Conformity D1Cb



**EC Declaration of Conformity**

We, **ProMinent Dosiertechnik GmbH**  
**Im Schuhmachergewann 5 - 11**  
**DE - 69123 Heidelberg**

hereby declare that, the product specified in the following complies with the relevant basic health and safety rules of the EC Directive, on the basis of its functional concept and design and in the version marketed by us. This declaration loses its validity in the event of a modification to the product not agreed with us.


Description of the product: **DULCOMETER Measuring and Control Device**

Product type: **D1Cc\_ \_ \_ X \_ \_ \_ \_ \_ \_ \_ \_ \_ \_ \_ \_ \_ \_**

Serial no.: **refer to nameplate overleaf and on the device**

Relevant EC Directives: **EC Low Voltage Directive (2006/95/EC)**  
**for characteristic value X=6**  
  
**EC EMC Directive (2004/108/EC)**  
**for characteristic value X = 4 or 6**

Harmonised standards applied, in particular: **EN 61010-1, EN 61326-1**

Date / manufacturer's signature: **09.03.2011** 

---

Details of the signatory: **Joachim Schall, Head of Development**

*Fig. 74: EC Declaration of Conformity D1Cc*

## 18 Index

<b>A</b>	
Access code.....	68
Activation code.....	55
Actuating outputs.....	76, 87
Actuator.....	124
Air humidity.....	141
Ambient conditions.....	141
<b>C</b>	
Cable end sleeves .....	29
Cable sheathing .....	29
Calibration.....	75
Caulk strip .....	27
Chemical Resistance.....	142
Complete operating menu.....	73
Control.....	126
Control panel installation.....	18, 41
Control panel mounting .....	25
Countersunk screws.....	28
<b>D</b>	
Delay period limits.....	123
Dimensions.....	143
DIN 43700.....	41
DIN EN 55014-1 EMC Requirements of household appliances Part 1 Emitted interference .....	150
DIN EN 55014-2 EMC Requirements of household appliances Part 2 Interference resistance .....	150
DIN EN 61010 Laboratory devices ...	150
DIN EN 61326 .....	150
Disposal.....	151
Drilling template .....	24
Dummy washer .....	29
<b>E</b>	
Environmental conditions.....	141
<b>F</b>	
Fixing material .....	24
Foam rubber .....	27
<b>G</b>	
General non-discriminatory approach....	3
General settings.....	131
<b>L</b>	
Limit exceeded.....	123
Limit relay.....	124
Limits.....	122
Lock nut .....	30
<b>M</b>	
Mains switch.....	19
mA-Output.....	129
Material Data.....	142
Material thickness .....	26, 41
Measured value.....	79
Measured variable.....	131
Measuring range.....	131
Membrane keypad.....	19
<b>N</b>	
Noise generation.....	141
non-discriminatory approach.....	3
<b>O</b>	
Operating Menu.....	67, 70, 82, 104
Overview.....	73
<b>P</b>	
Parameter.....	67, 70, 82, 104
Parked position.....	28
plant rooms.....	142

Polyester PET membrane.....	142	Storage conditions.....	141
PPE-GF10.....	142	Switching times.....	121
PPE-GF20.....	142	<b>T</b>	
Pressure ring .....	29	Terminal diagram.....	44
Projection of device .....	27	Terminal wiring diagram .....	30
Protective low voltage .....	21	Theoretical switching time.....	121
Punched template .....	25	Timer.....	119
<b>R</b>		Timer relay.....	119
Ribbon cable.....	19	<b>U</b>	
Run-in times.....	76, 87	User inputs.....	19
<b>S</b>		Users' qualifications.....	10
Safety information.....	8	<b>W</b>	
Seal .....	29	Wall bracket .....	24
Sensor function.....	76, 87	Wall mounted.....	18, 24
Setting menus.....	68	Wall plug .....	24
Solenoid valves.....	119	Weights.....	143
Sound Pressure Level.....	141	<b>Z</b>	
Spare parts.....	148, 149	Zero point calibration.....	76
Standard signal outputs.....	76, 87		